




# *Possibilities and plans for materials research using neutron beams at the MARIA Reactor*



NARODOWE  
CENTRUM  
BADAŃ  
JĄDROWYCH  
ŚWIERK

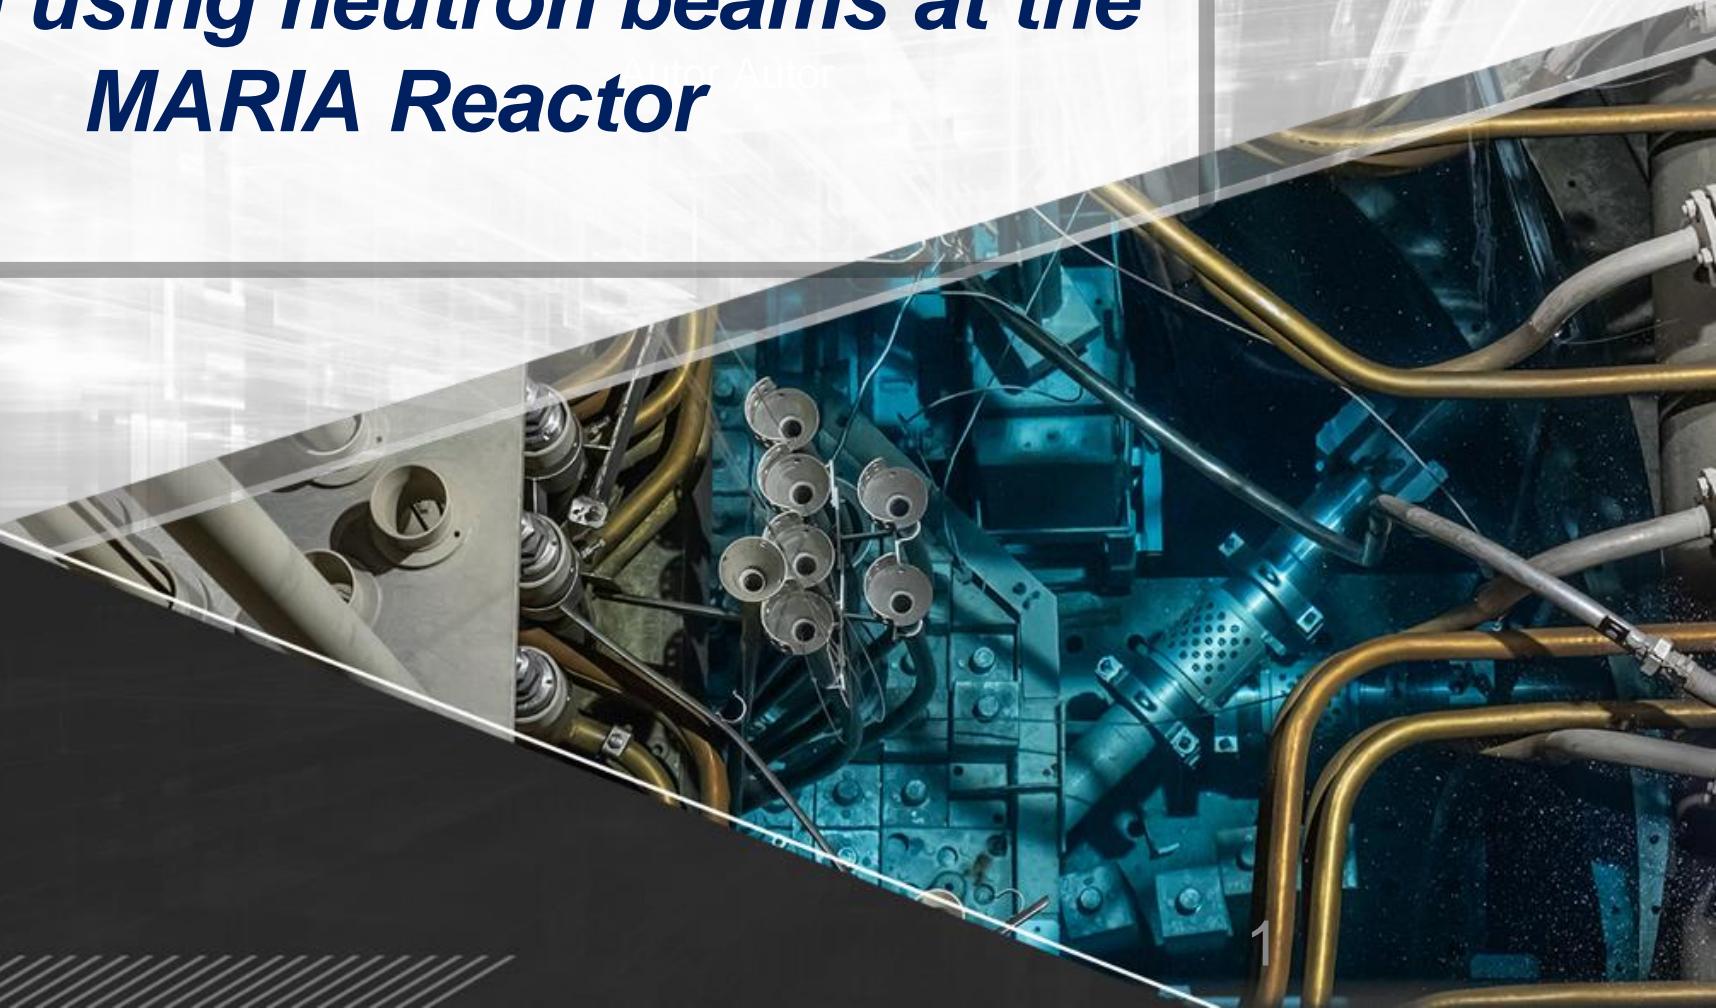


# **Outline:**

- ***The MARIA Reactor***
- ***Experimental hall***
- ***MARIA NEUTRON LABORATORY MNL***
- ***Instruments***
- ***Preparations for the creation of the MNL laboratory***

# *National Centre for Nuclear Research*

## *Narodowe Centrum Badań Jądrowych (NCBJ)*

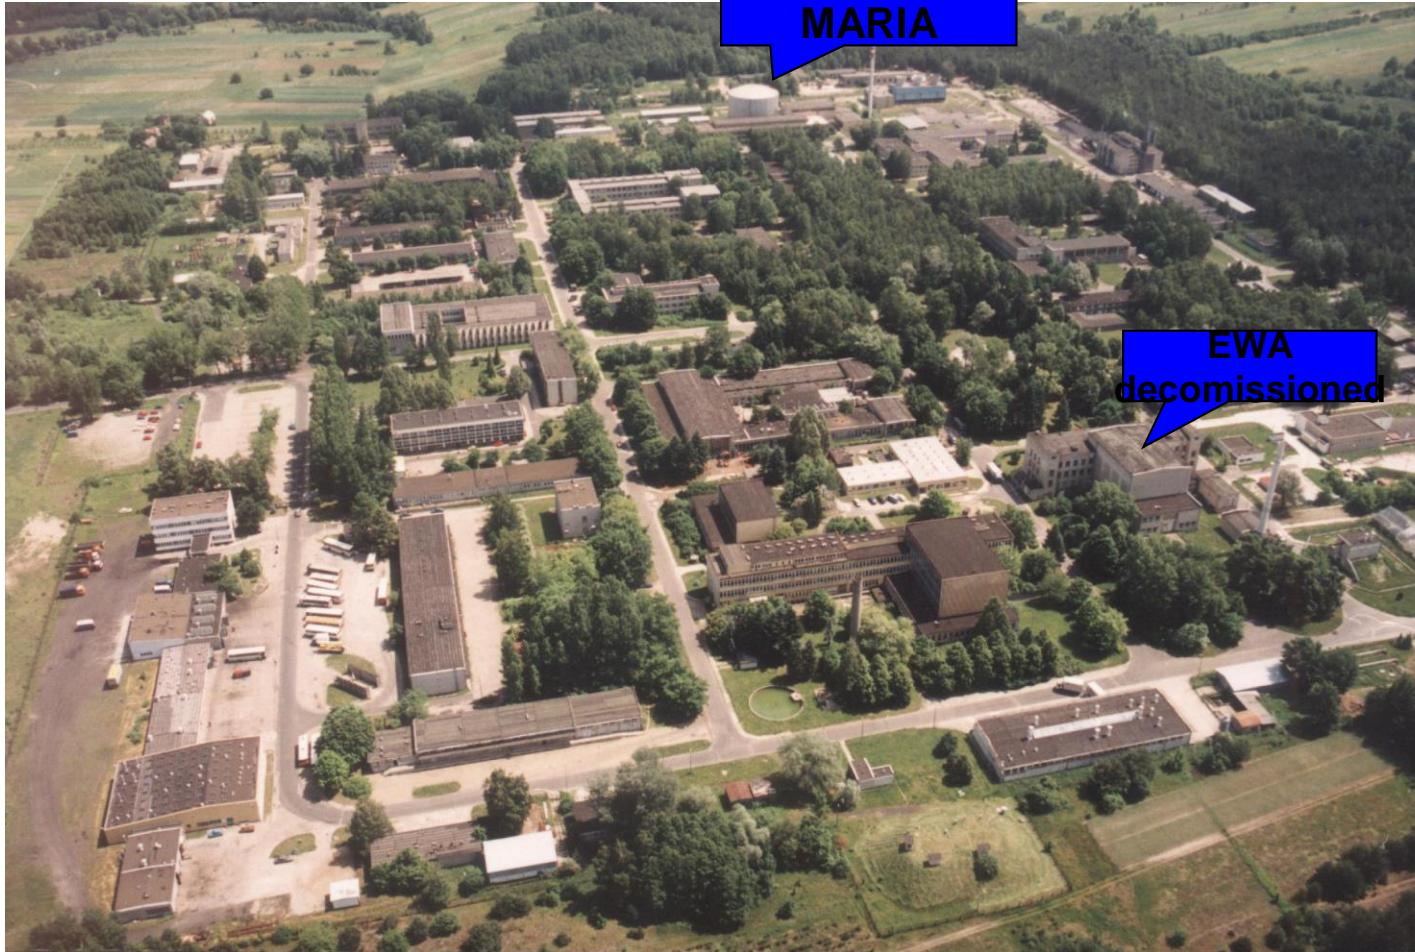

# MARIA Reactor


<b>Reactor type</b>	pool-type reactor with pressurized fuel channels
Start operation	1974
Thermal power	Max. 30 MW,
Nominal power	19-26 MW
Fuel	MC-5 19,7 % 485 g U-235 $\text{U}_3\text{Si}_2$ MR-6 19,75 % 485 g U-235 $\text{UO}_2\text{-Al}$
Thermal neutron flux	$2,5 \times 10^{14} \text{ n/cm}^2\cdot\text{s}$
Fast neutron flux	$2 \times 10^{14} \text{ n/cm}^2\cdot\text{s}$
Moderator	$\text{H}_2\text{O}$ ; beryllium
Reflector	graphite
Licence	2025, Relicensing to ....




# **Current main reactor applications:**

- *production of radioisotopes,*
- *testing of fuel and structural materials for nuclear power engineering,*
- *neutron transmutation doping of silicon,*
- *neutron modification of materials*
- *research in neutron and condensed matter physics*
- *neutron radiography,*
- *neutron activation analysis,*
- *neutron beams in medicine*
- *training in the field of reactor physics & technology.*

# MARIA Reactor

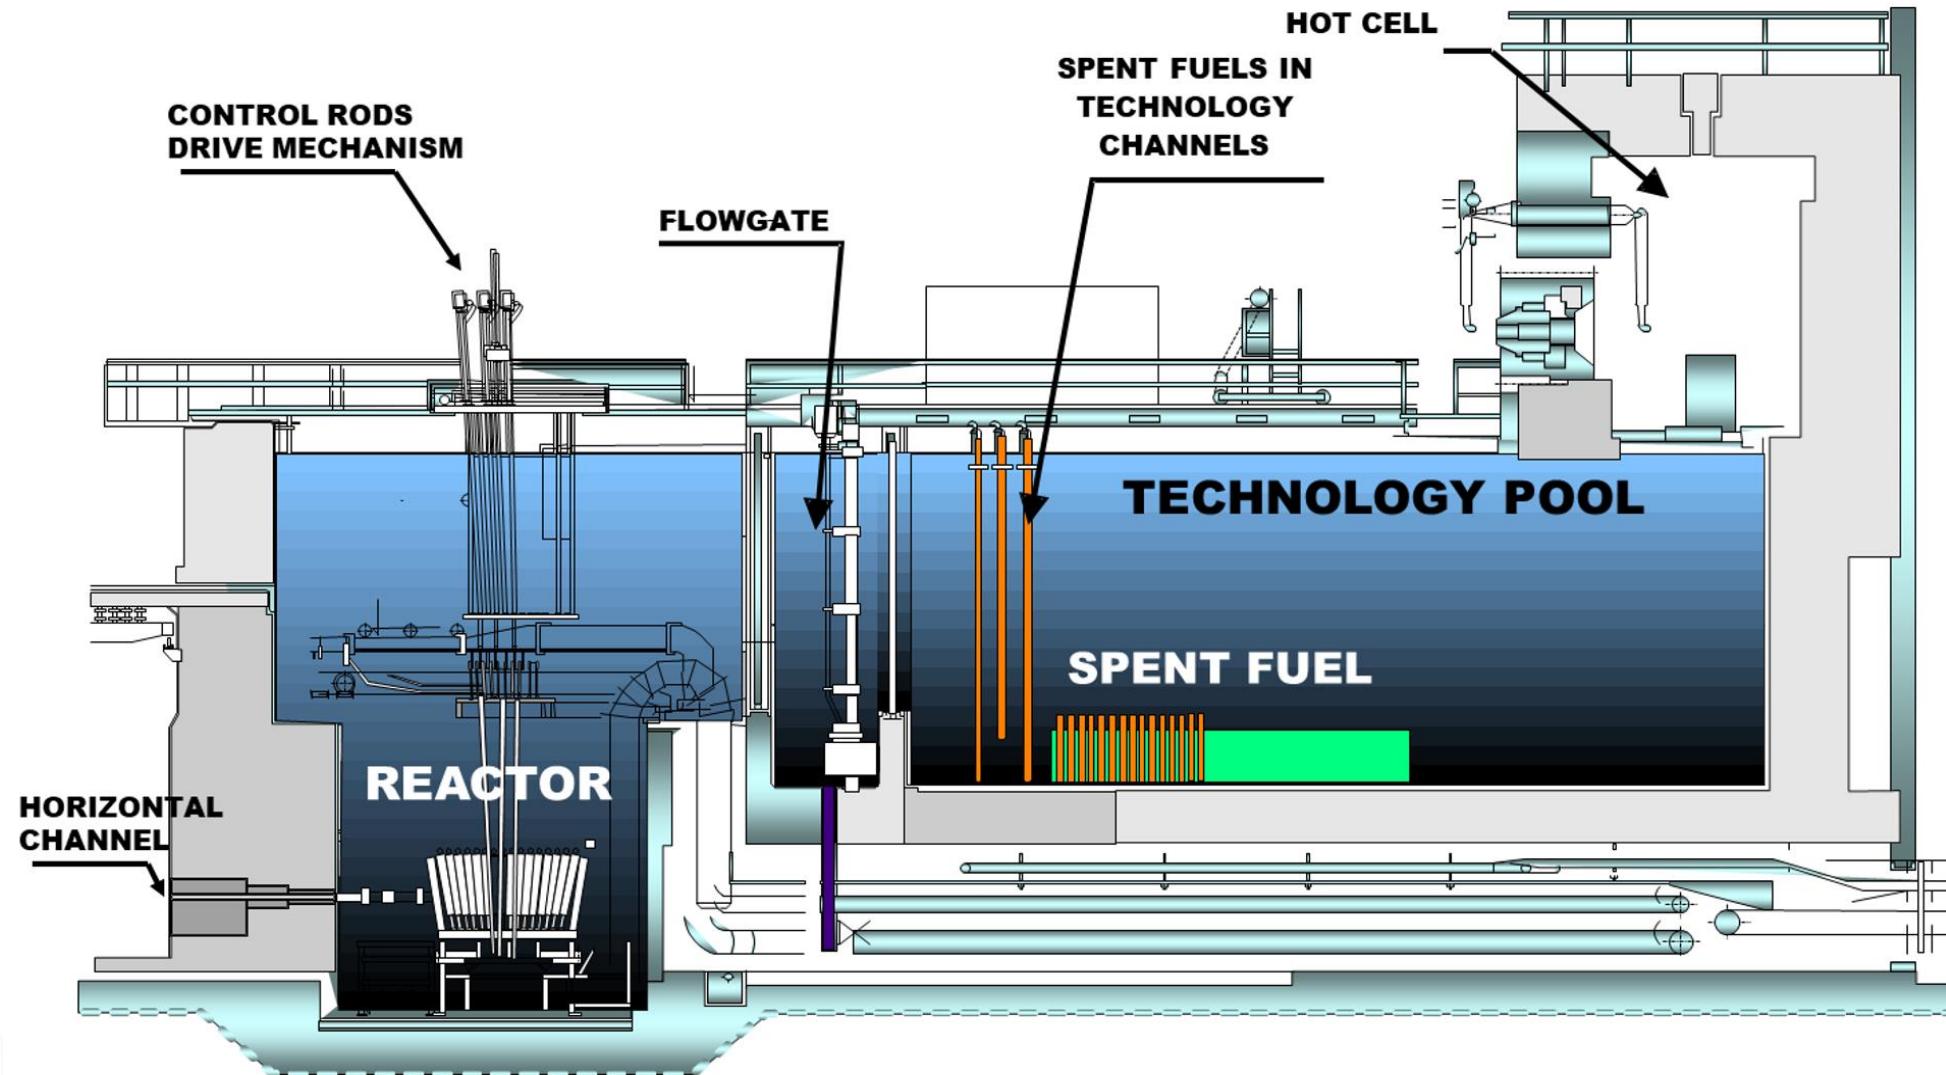

# NRR MARIA cross-section

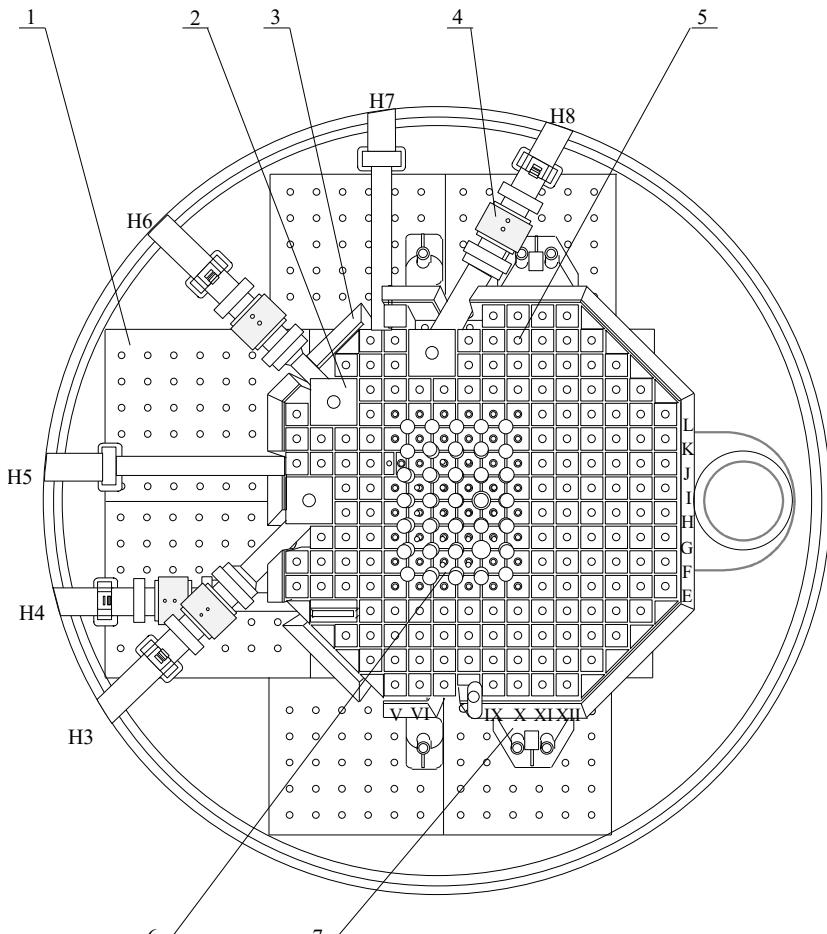


1. core and reflector support plate
2. multiple graphite block
3. reflector support structure
4. beam tube compensator joint

5. graphite reflector block
6. beryllium block
7. ionization chambers shield

## Horizontal neutron beams

**Thermal neutrons flux  
at horizontal neutron beams  
outlets**

$$4 \times 10^9 \text{ cm}^{-2} \text{ s}^{-1}$$

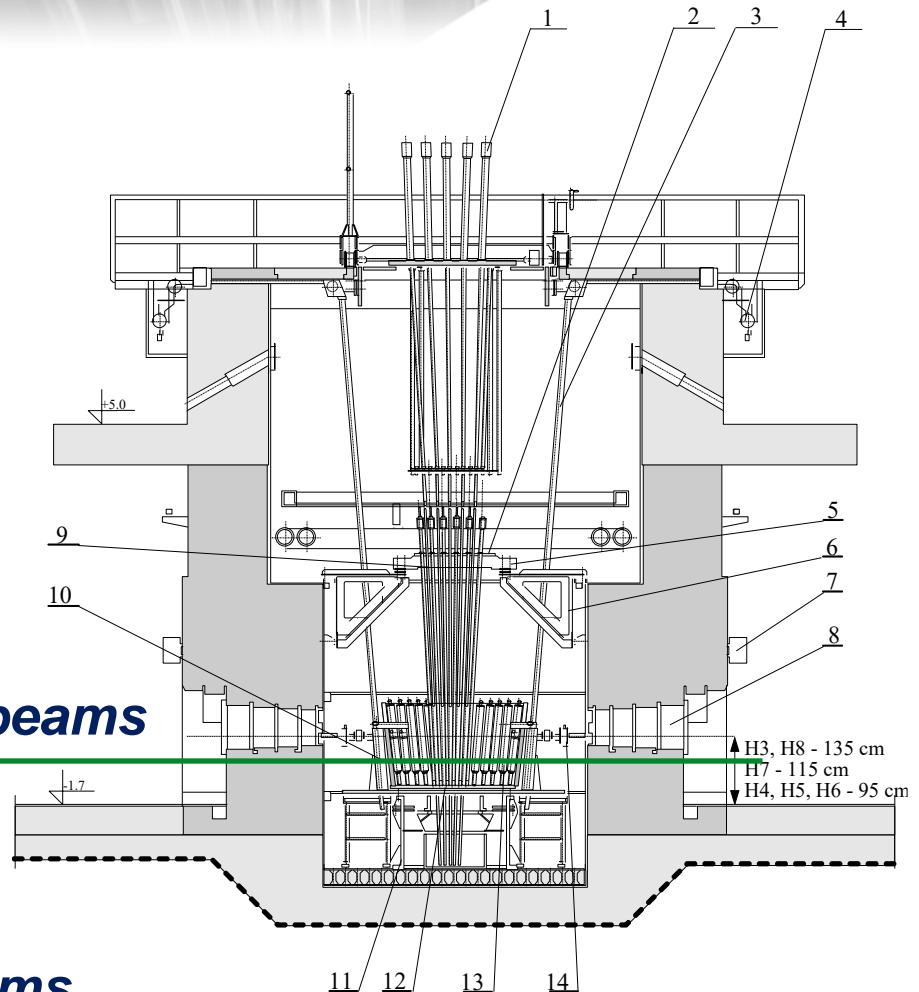


1. control rod drive mechanism
2. mounting plate
3. ionization chamber channel
4. ionization chamber drive mechanism
5. fuel and loop channels support plate
6. plate support console
7. horizontal beam tube shutter drive mechanism
8. beam tube shutter
9. fuel channel
10. ionization chambers shield
11. core and support structure
12. core and reflector support plate
13. reflector blocks
14. beam tube compensator joint

*The experimental hall  
of neutron scattering laboratory  
before 2017 comprised  
7 thermal neutron instruments:*

- *2 neutron spectrometers*
- *2 neutron diffractometers*
- *2 small angle scattering (SANS) diffractometers*
- *Neutron/gamma radiography – tomography facility*


# EXPERIMENTAL HALL before 2017

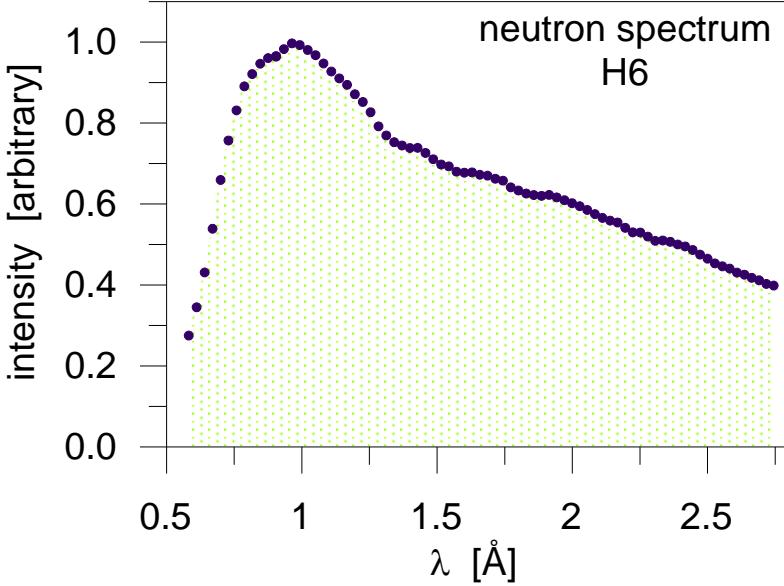

TAS

NR

neutron flux density at the sample  $\sim 5 \times 10^5 \text{ cm}^{-2} \text{ s}^{-1}$

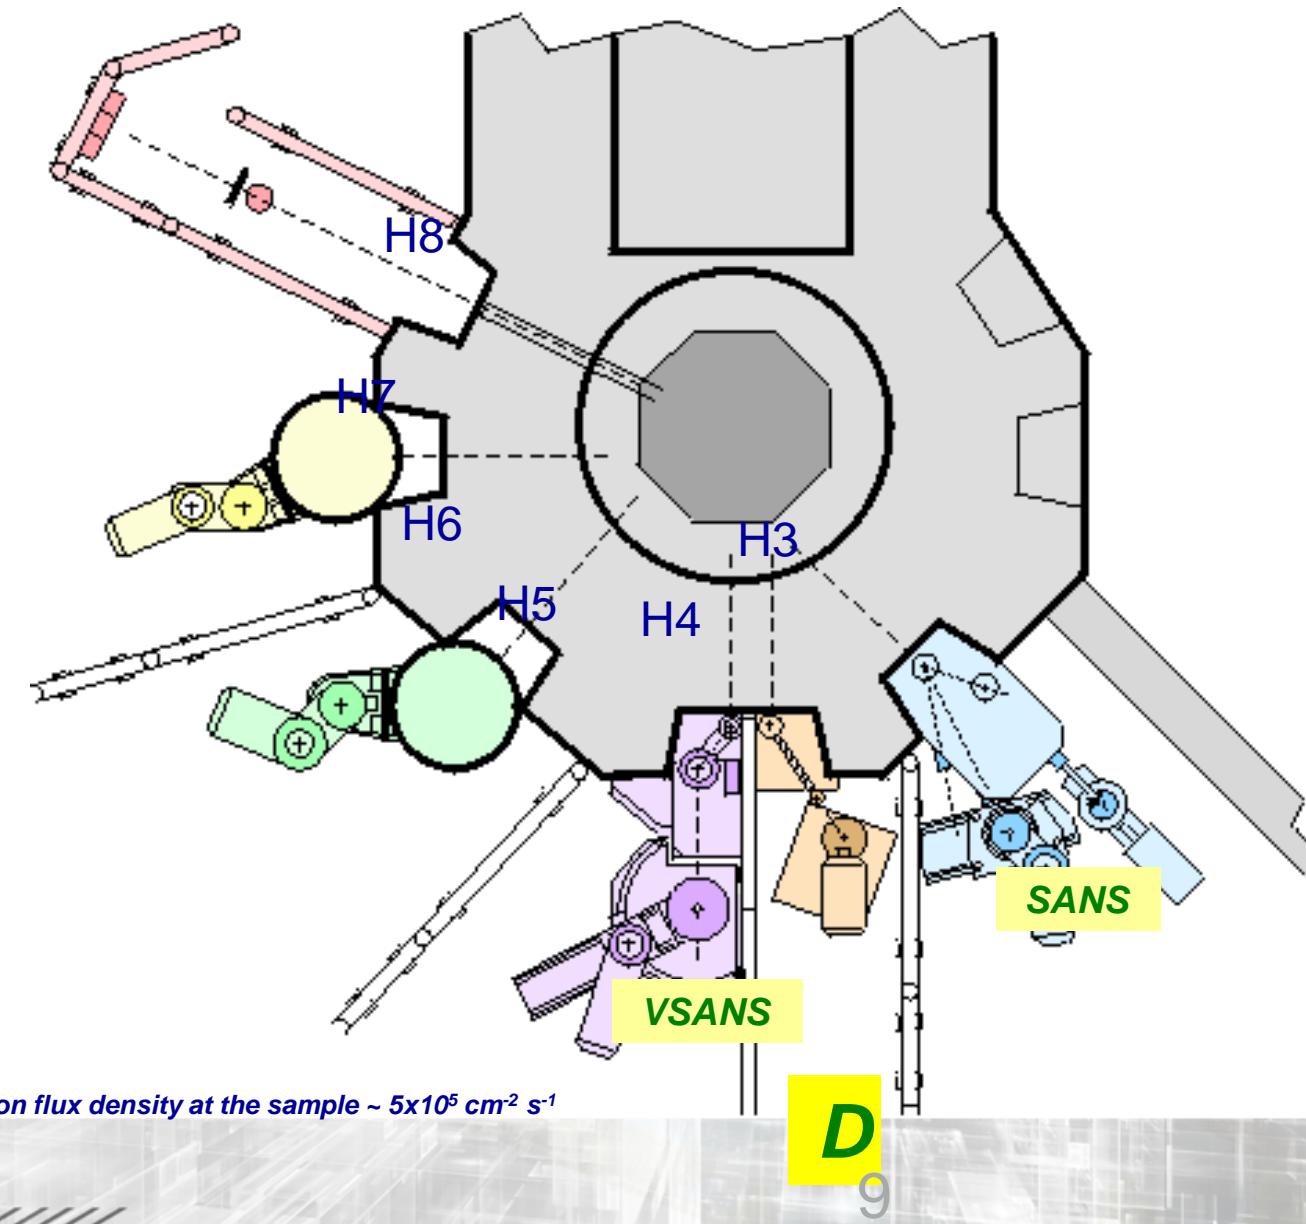

# EXPERIMENTAL HALL before 2017



*Since 2021 the experimental hall @ MARIA NRR has been refurbished for five HZB thermal neutron instruments*

## **MARIA NEUTRON LABORATORY MNL**

*Open access on the application competition*

# HZB MACHINES


*E2 - Flat Cone Diffractometer,*

*E3 – Residual Stress Analysis Diffractometer,*

*E4 – Two-Axis Diffractometer,*


*E5 - Four-Circle Diffractometer,*

*E6 – Focusing Diffractometer.*


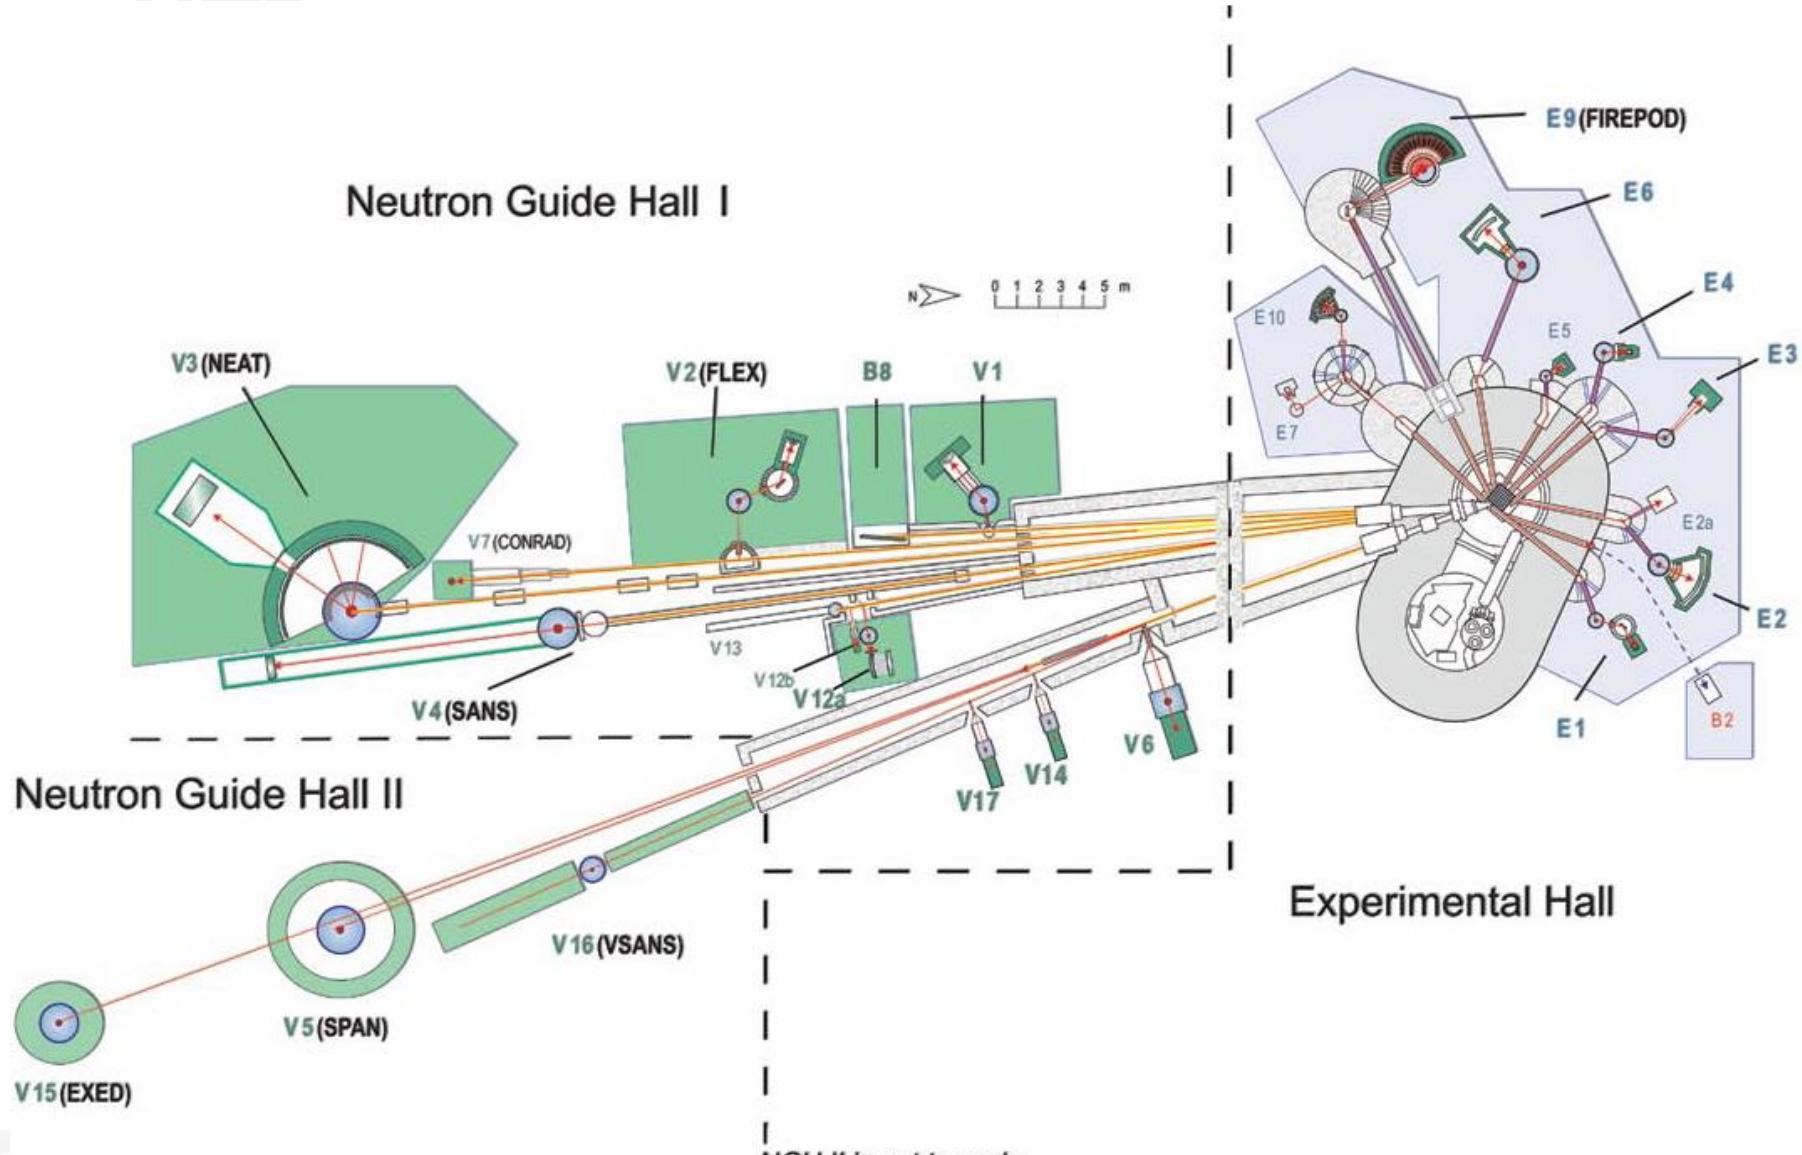


**Neutron Scattering Instrumentation  
at the Research Reactor BER II**  
Berlin Neutron Scattering Center – BENSC, 2007

## PLANNED ARRANGEMENT @ THE MARIA EXPERIMENTAL HALL

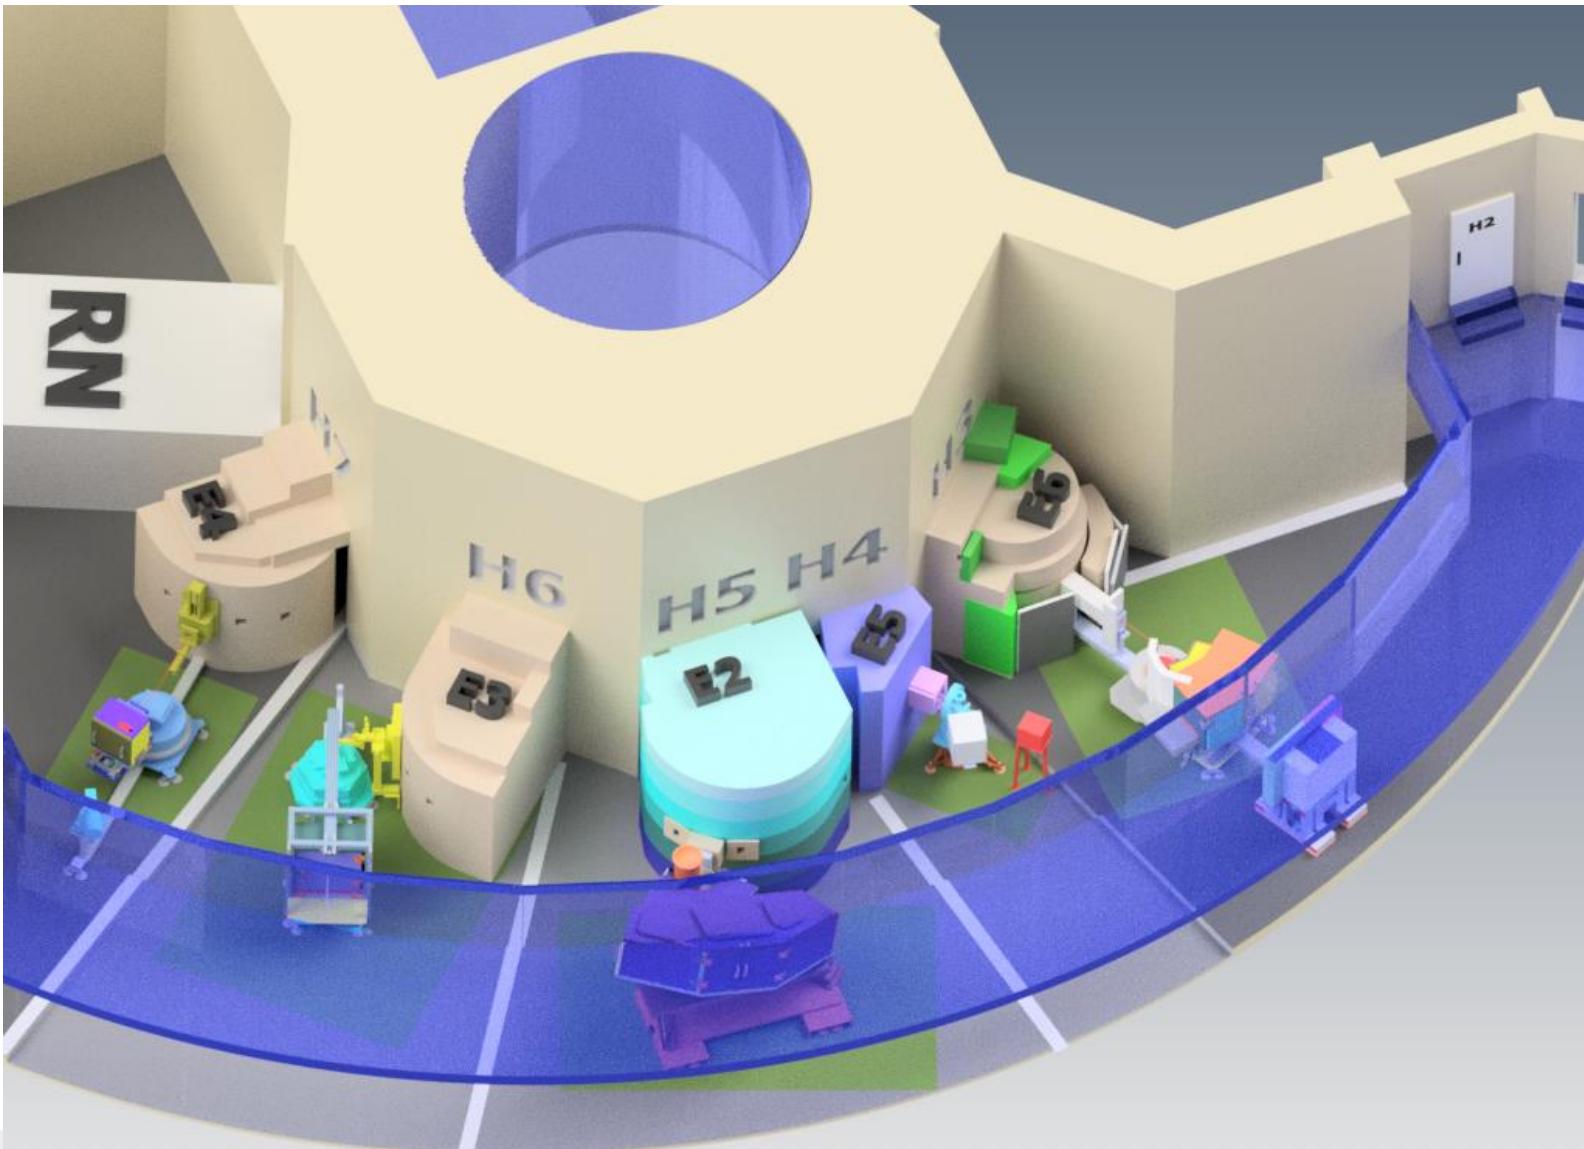

## PLANNED ARRANGEMENT @ THE MARIA EXPERIMENTAL HALL

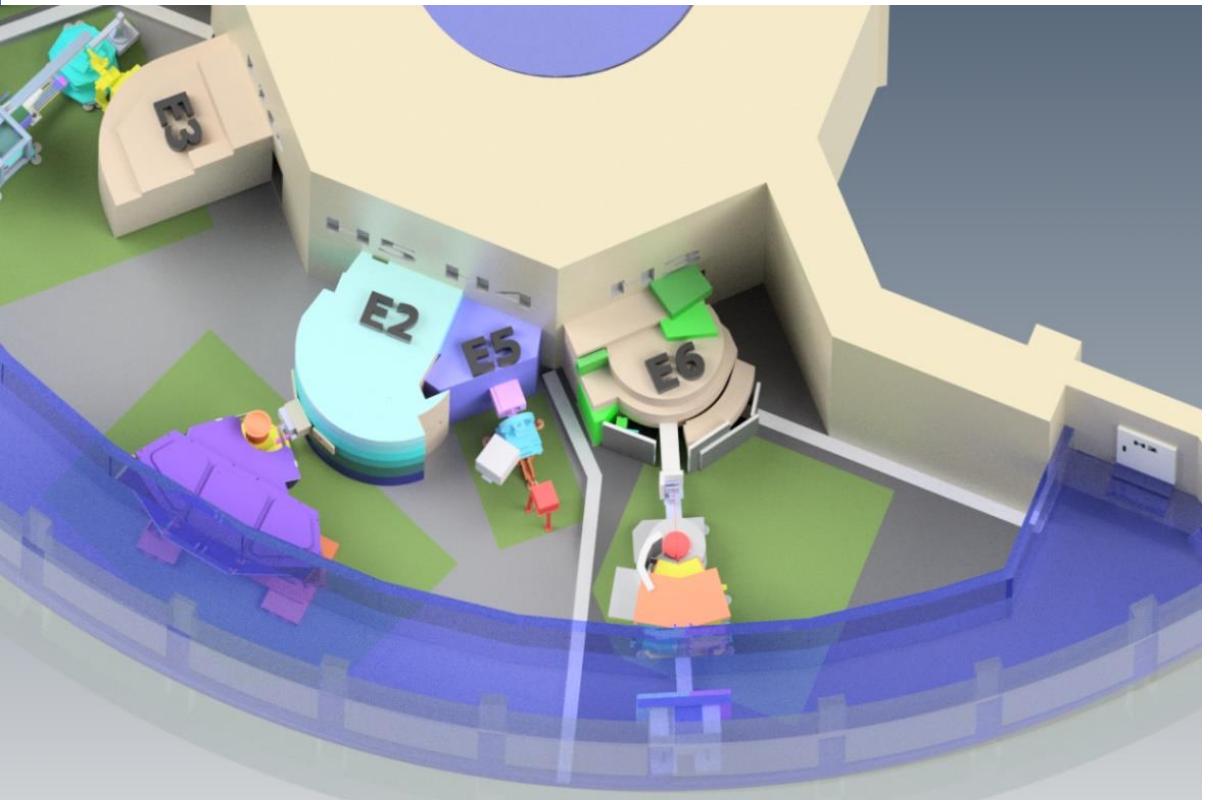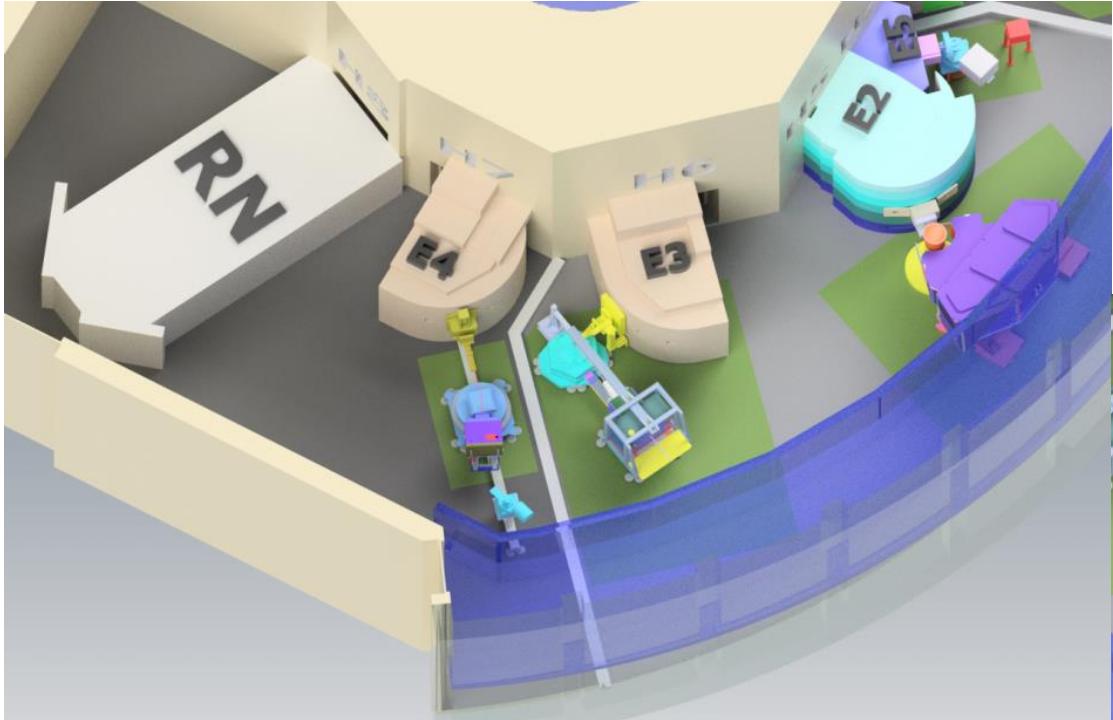

**All diffractometers are equipped with 2-dimensional position sensitive  
 $\text{He}^3$  neutron detectors and focusing monochromators**

**E2. Flat cone diffractometer**

*Monochromator Cu (220),  $\lambda=0.91 \text{ \AA}$  Ge (311),  $\lambda=1.21 \text{ \AA}$ , PG (002),  $\lambda=2.41 \text{ \AA}$ ;  
4 x 2D PSD 30 x 30 cm*

**E3. Diffractometer for Microstructure and Residual Stress Analysis**

*Monochromator Si (400), Double focusing,  $\lambda = 1.48 \text{ \AA}$ ; 2D PSD 30 x 30 cm*

**E4. Two-Axis Diffractometer.**

*Monochromator PG (002):  $\lambda = 2.4 \text{ \AA}$  or Ge (113):  $\lambda = 1.2 \text{ \AA}$ ; 2D PSD 20 x 20 cm*


**E5. Four-Circle Diffractometer.**

*Monochromator Cu(220);  $\lambda = 0.9 \text{ \AA}$  or PG(002),  $\lambda = 2.4 \text{ \AA}$ , PSD 9 x 9 cm*

**E6. Focusing Diffractometer.**


*Monochromator PG (002)  $\lambda = 2.4 \text{ \AA}$  double focusing, two 2D PSD each 30 x 30 cm*

## **E2 diffractometer - Possibility of tilting the detector from the horizontal scattering plane**


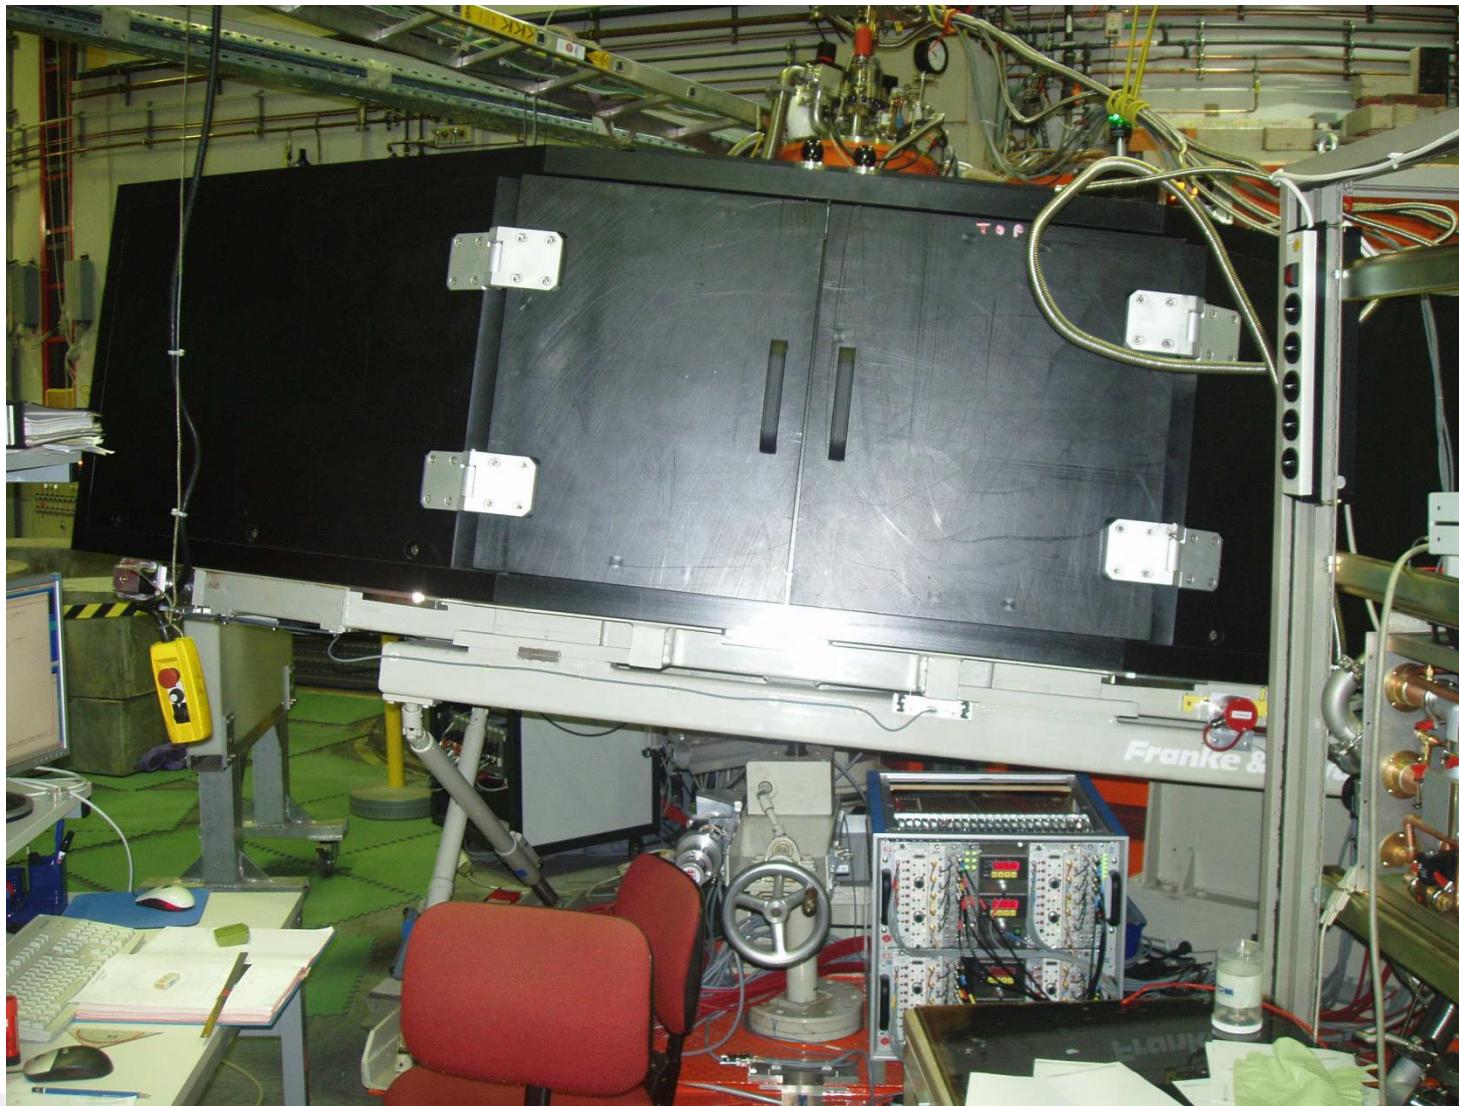


[https://www.helmholtz-berlin.de/pubbin/igama\\_output?modus=datei&did=628](https://www.helmholtz-berlin.de/pubbin/igama_output?modus=datei&did=628)



## E2 diffractometer

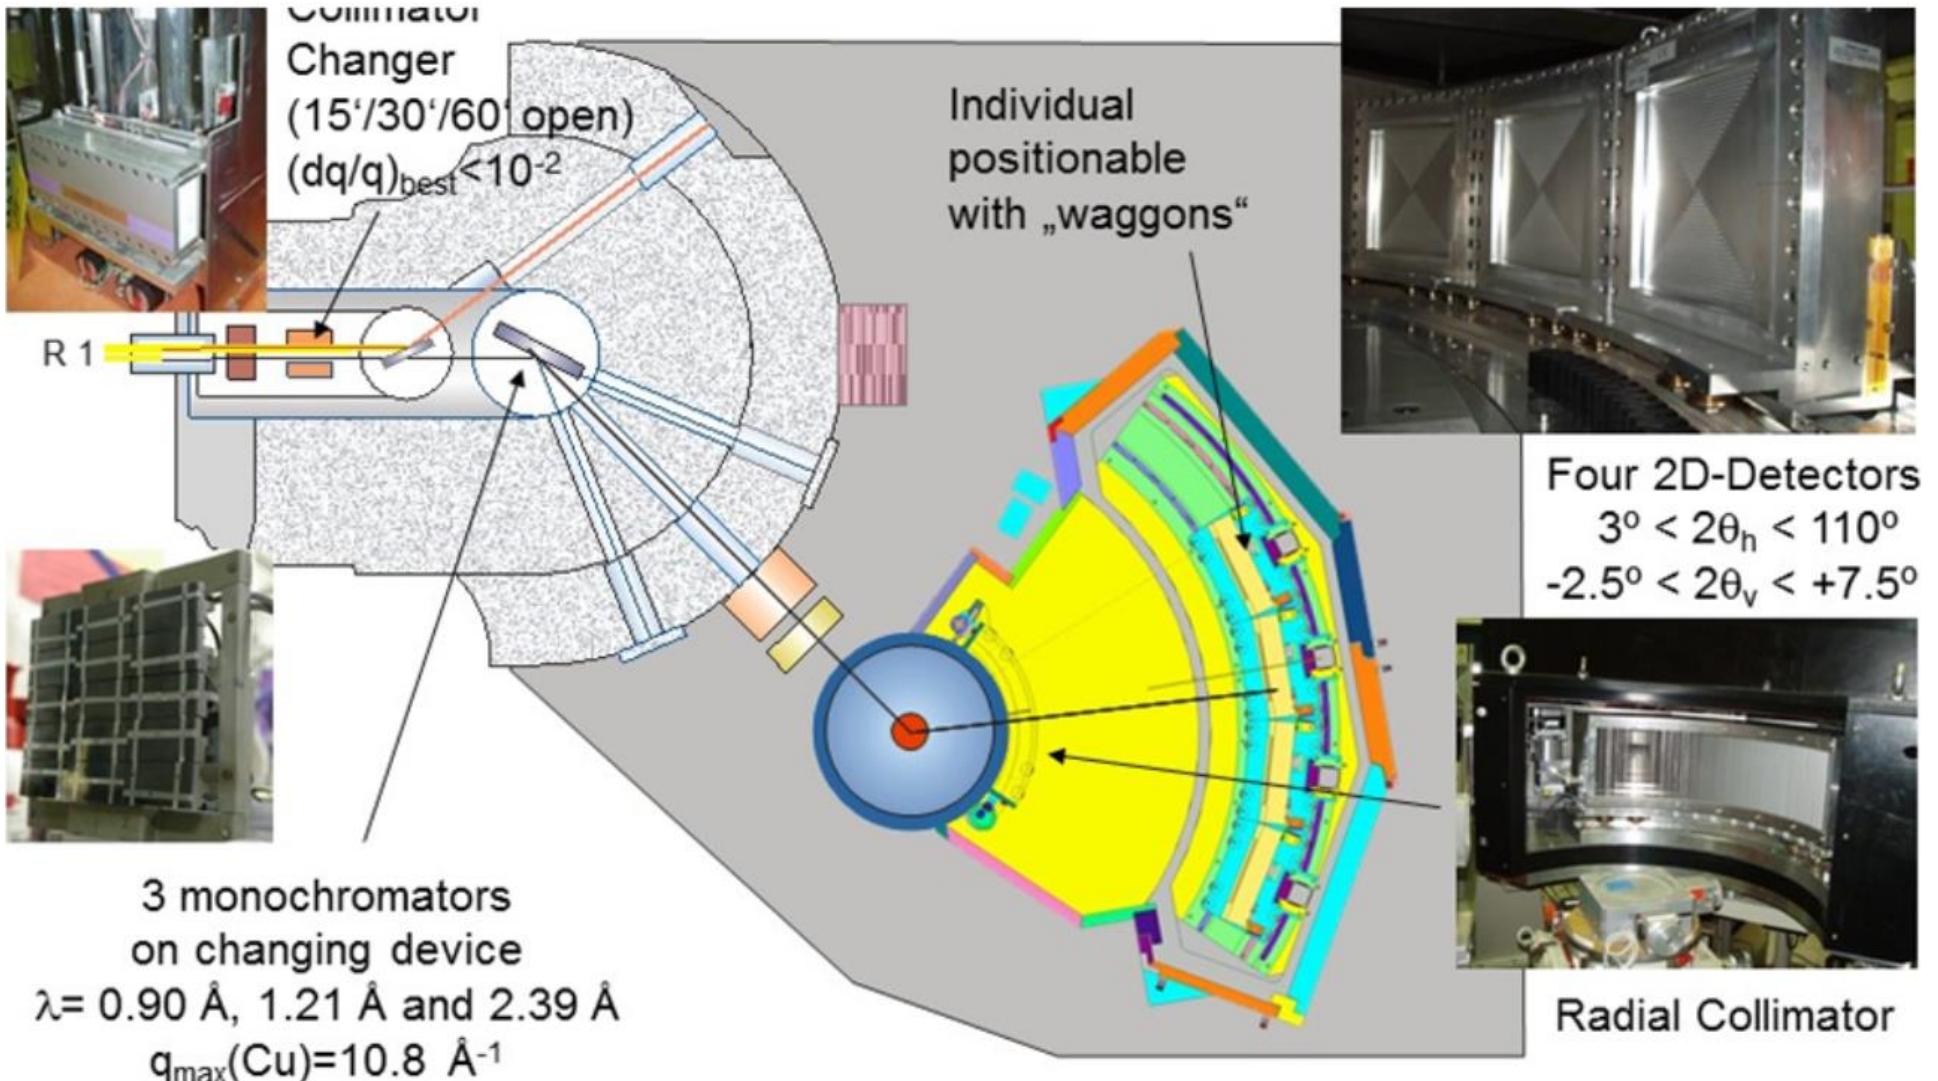


## **E3 diffractometer for internal stress studies in macroscopic elements**

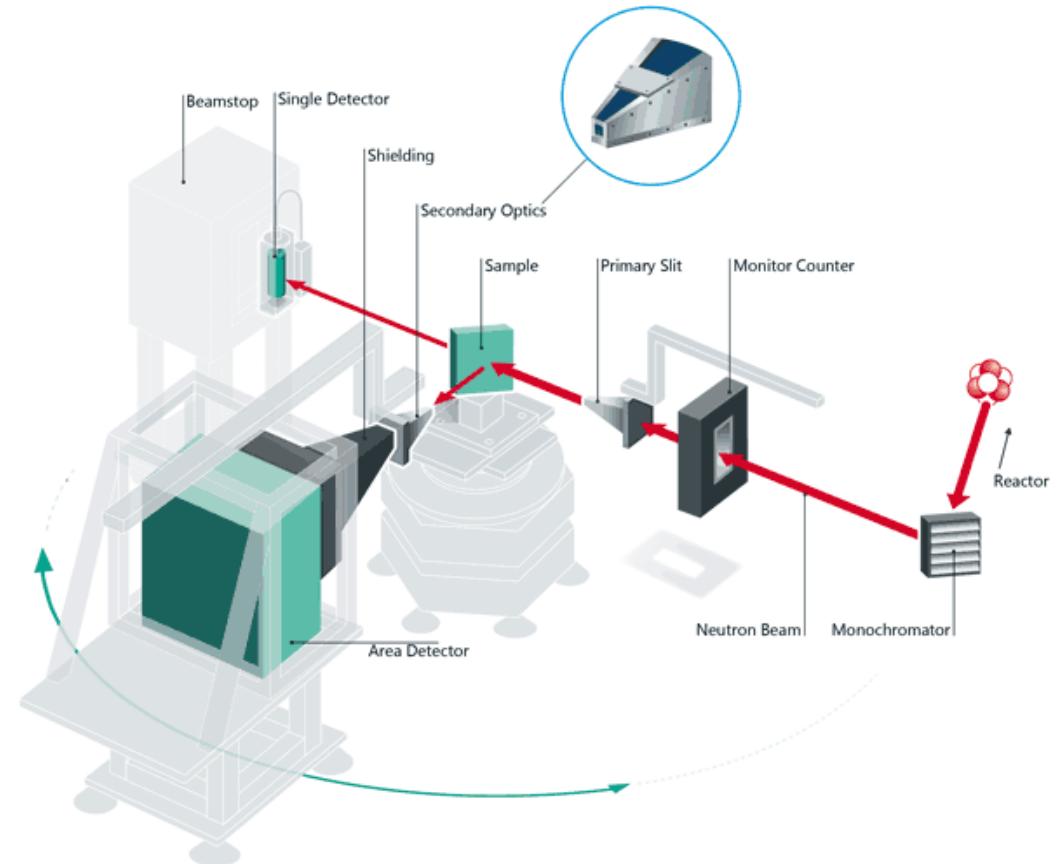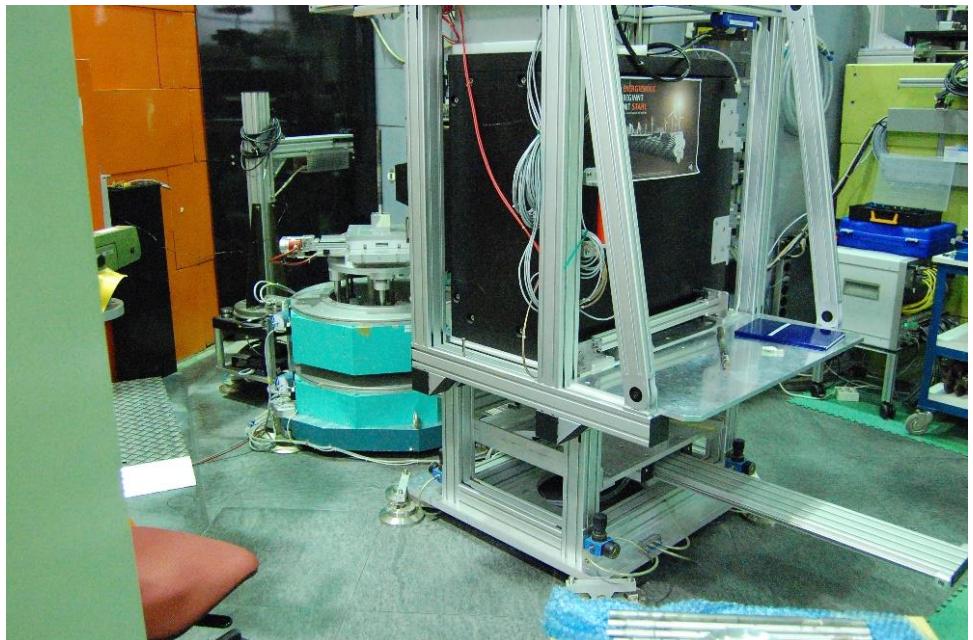


## *E3 diffractometer*

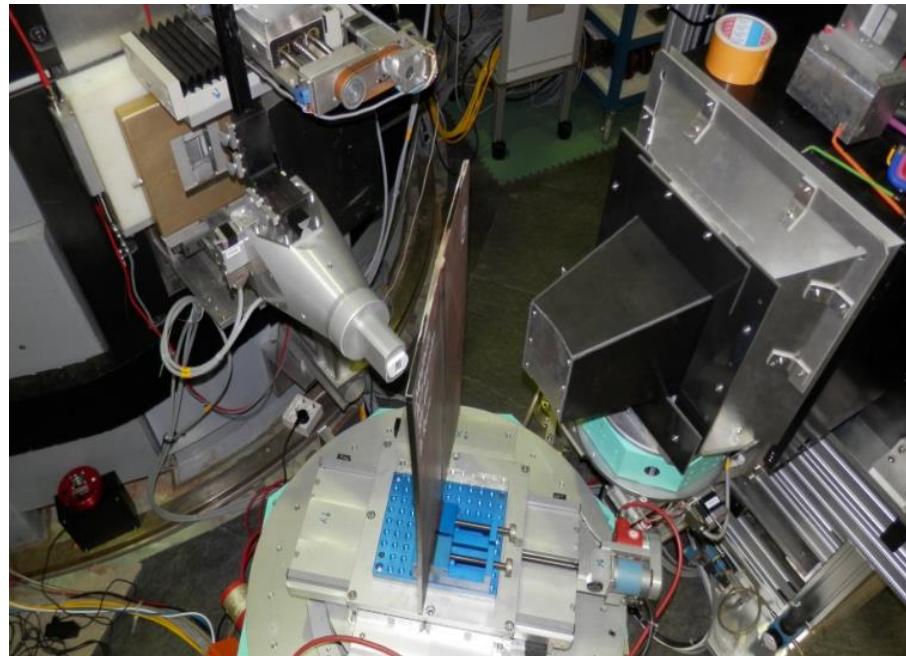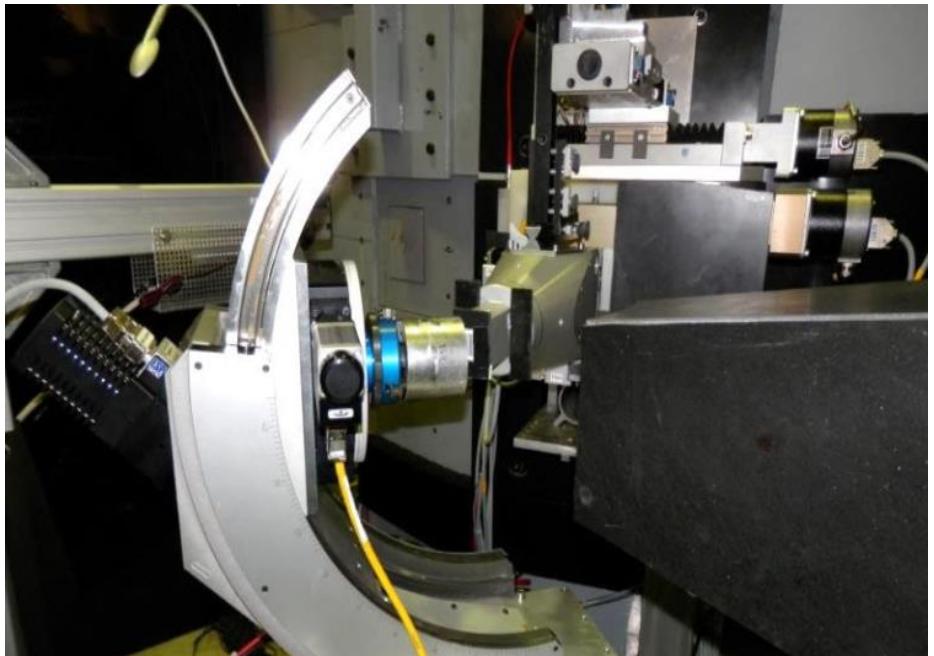

## E4 diffractometer

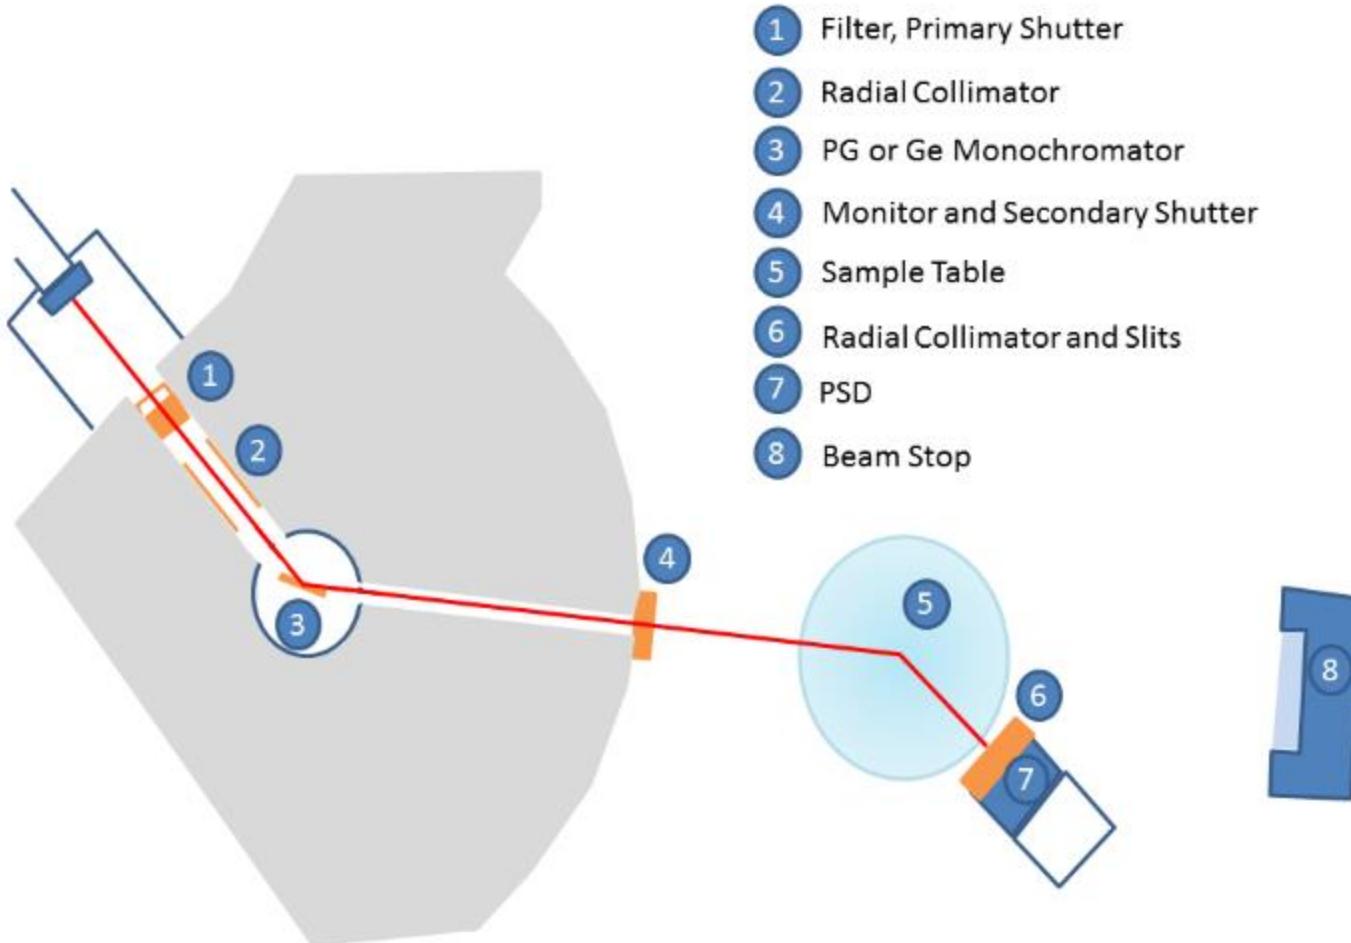


## *E4 diffractometer*

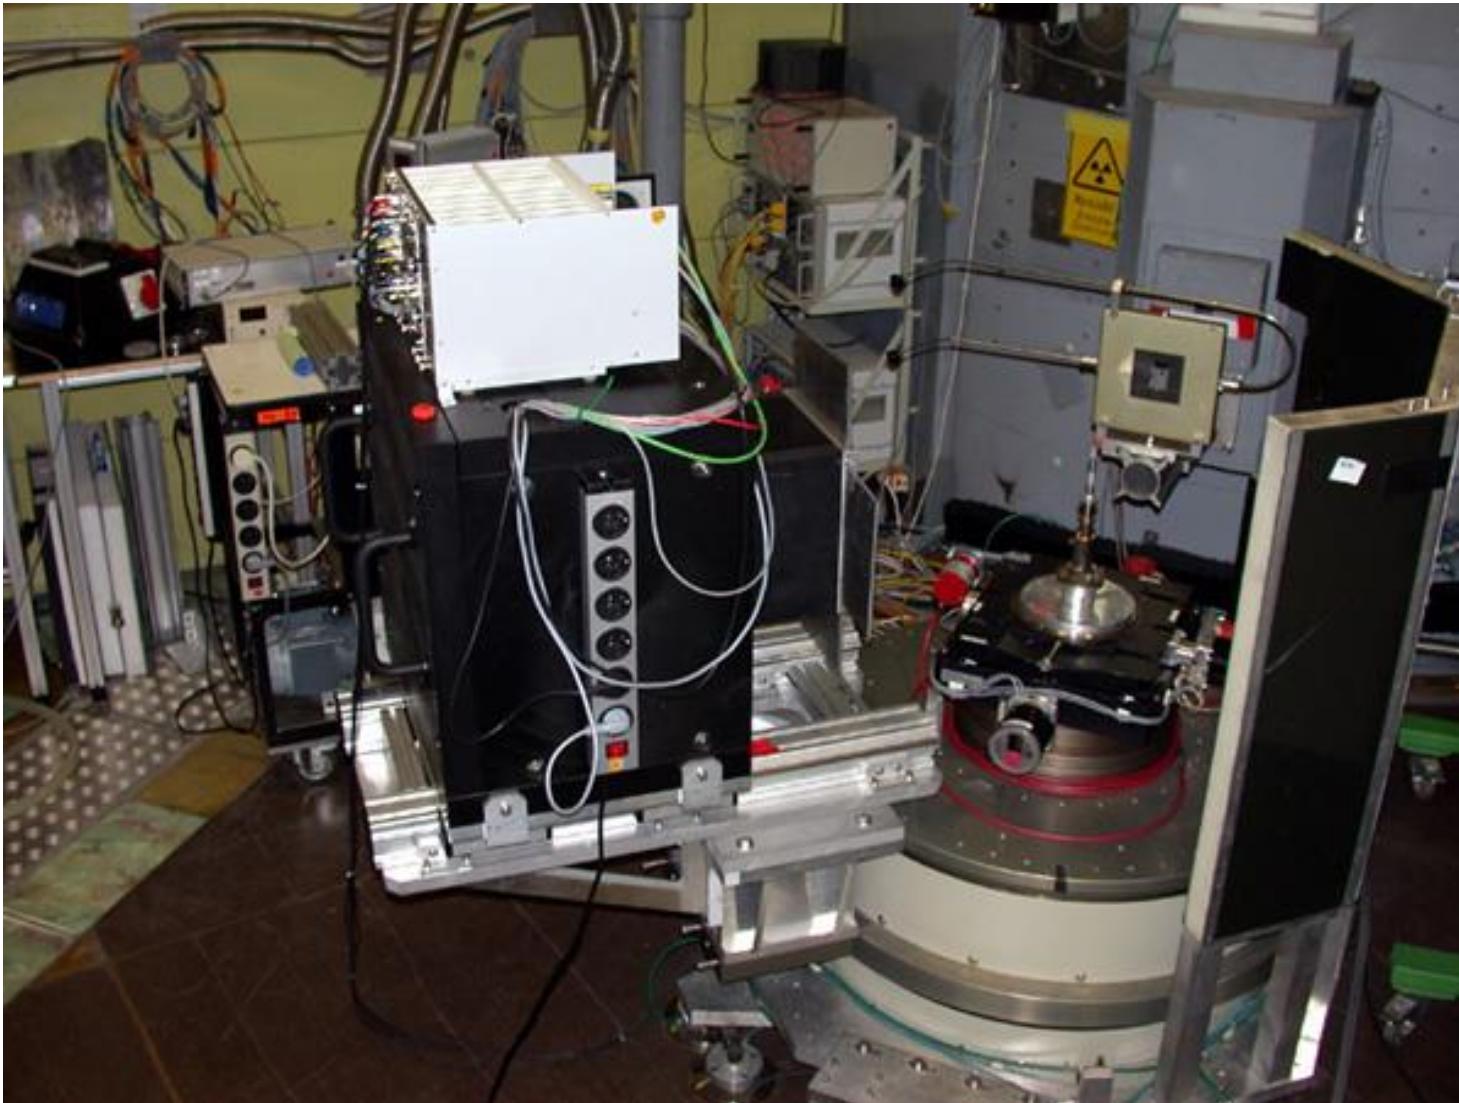


[https://www.helmholtz-berlin.de/pubbin/igama\\_output?modus=einzel&gid=1699](https://www.helmholtz-berlin.de/pubbin/igama_output?modus=einzel&gid=1699)

## E5 diffractometer

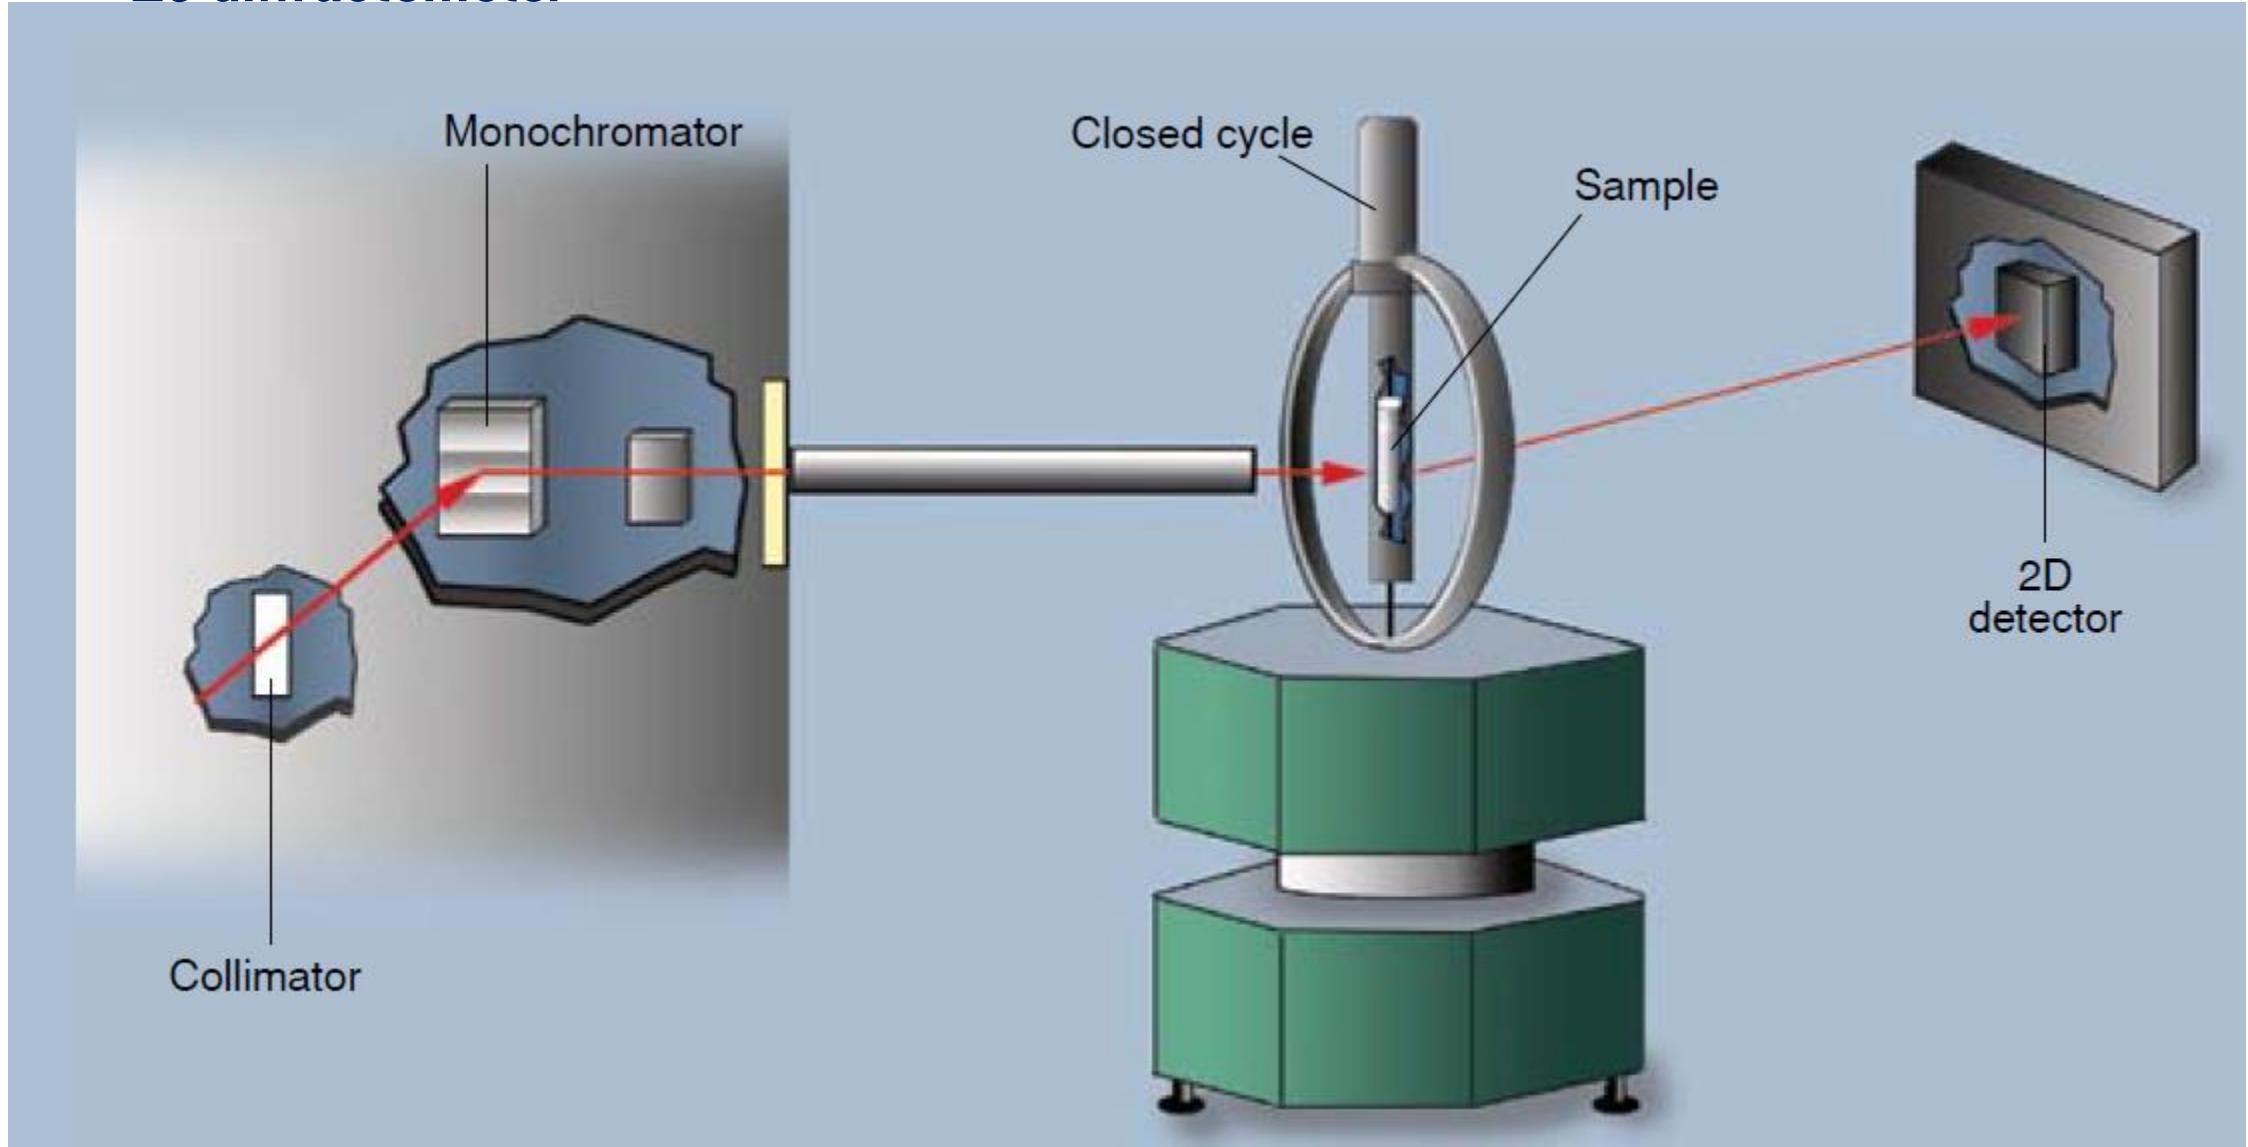


Neutron Scattering Instrumentation at the Research Reactor BER II  
Berlin Neutron Scattering Center – BENSC, 2007

## *E6 diffractometer*


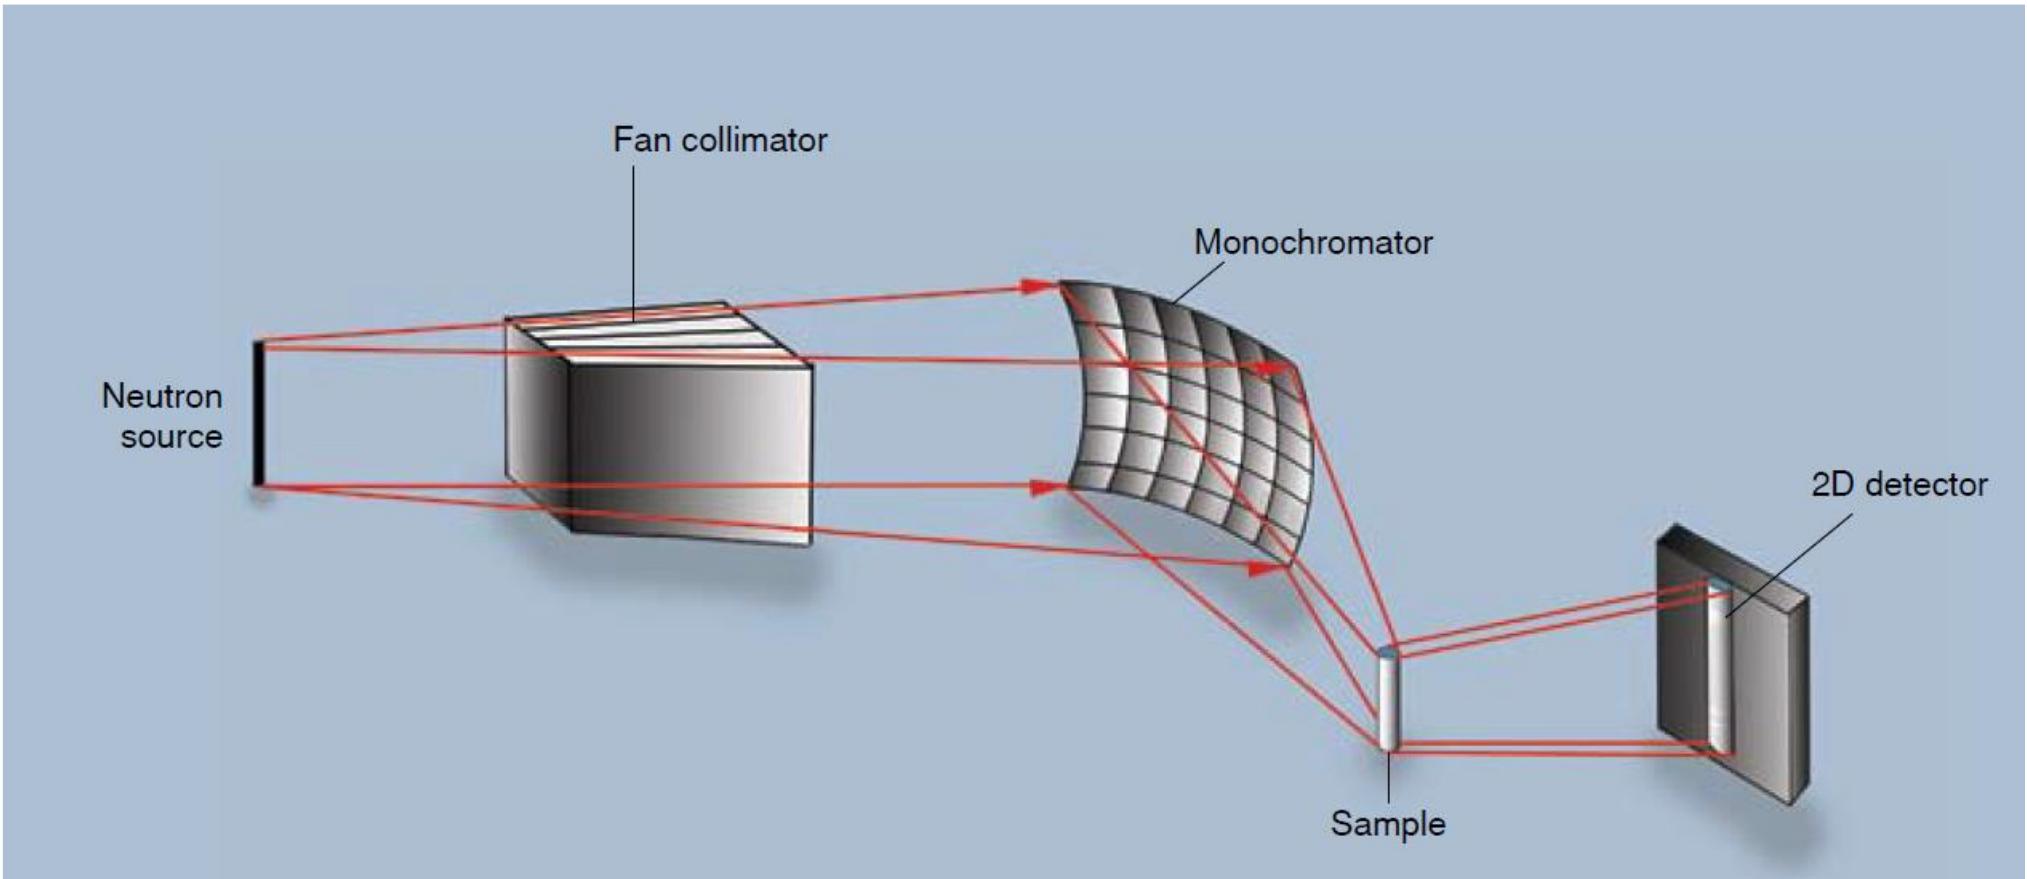


## *E6 diffractometer*

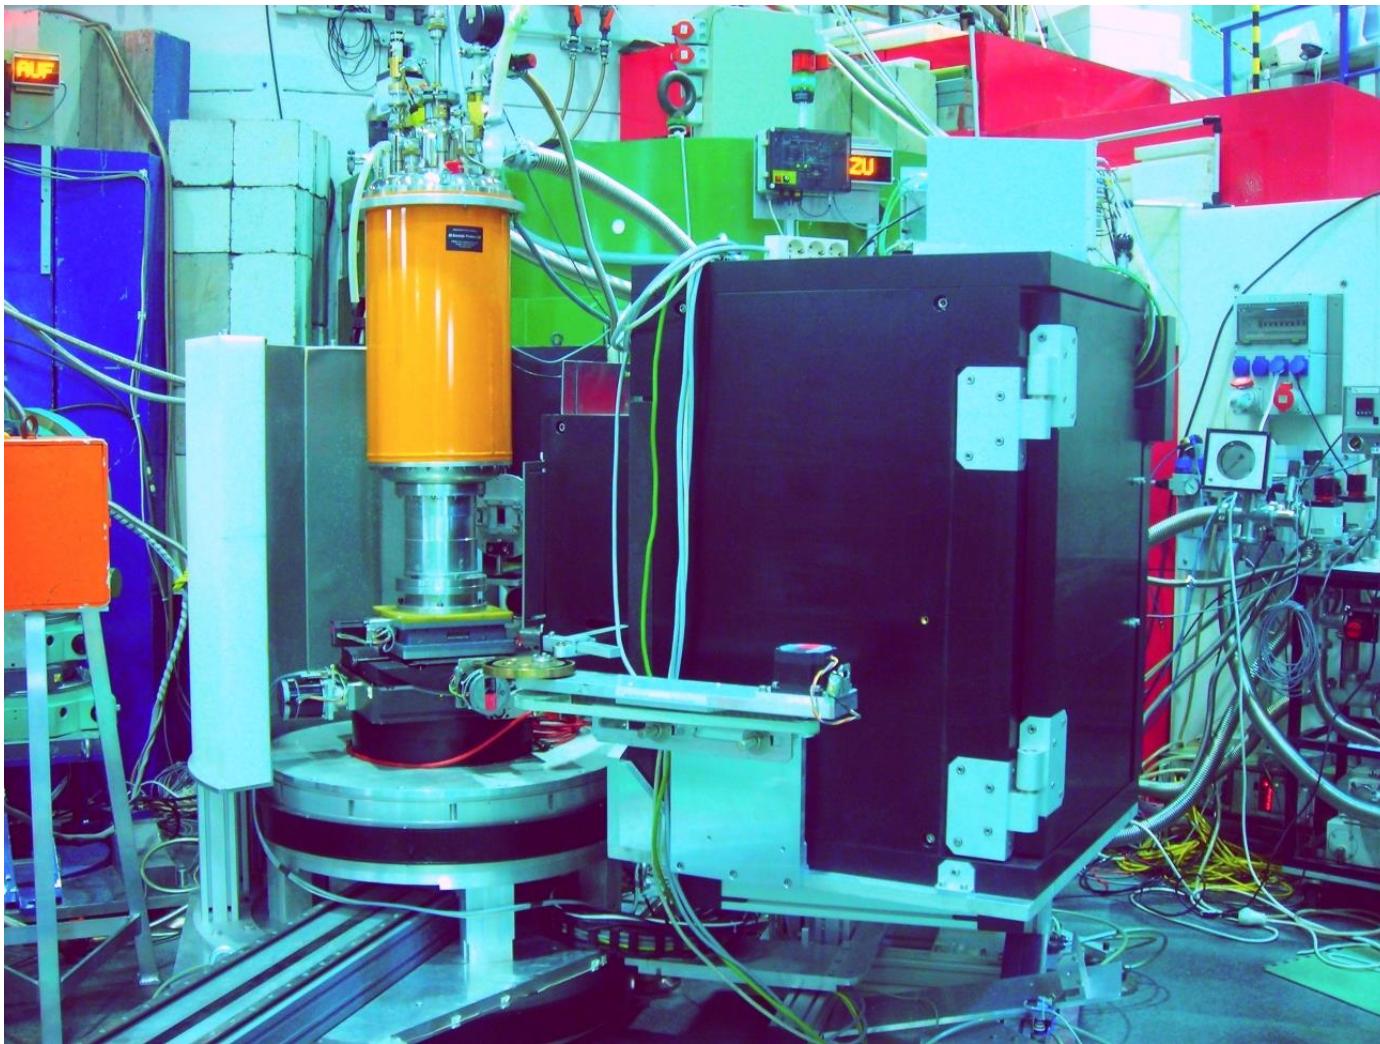

**Neutron Scattering Instrumentation at the Research Reactor BER II**  
Berlin Neutron Scattering Center – BENSC, 2007

## H8 neutron radiography station

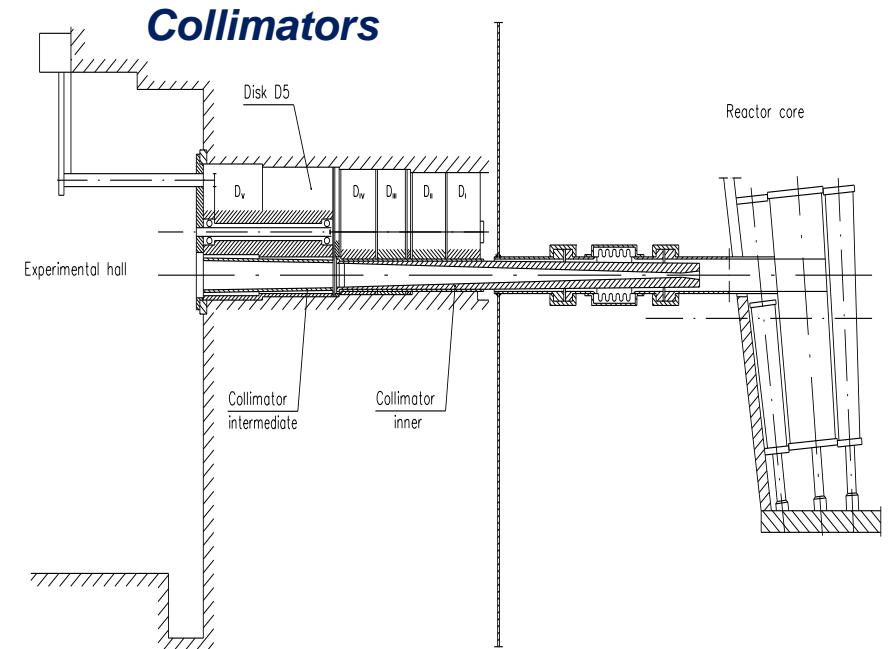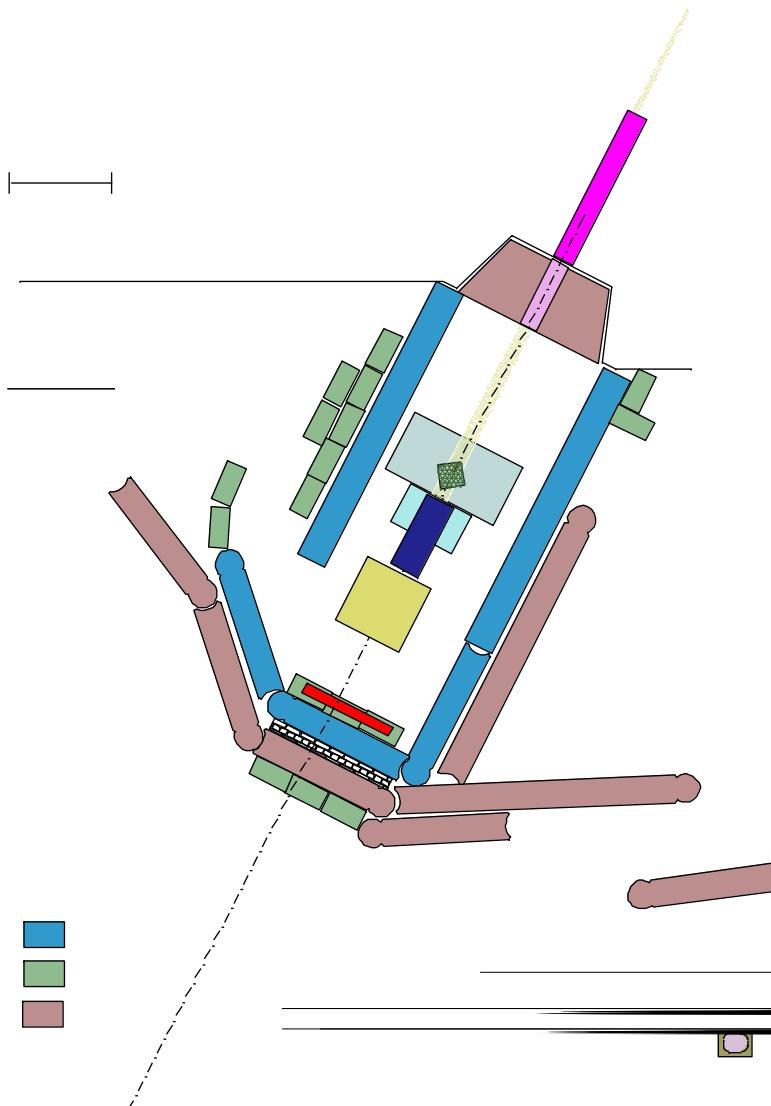

## ***Neutron Radiography facility main parameters***

**$100 < L/D < 200$**

**neutron flux density =  $1.1 \times 10^7 \text{ n cm}^{-2} \text{ s}^{-1}$  (at L/D = 150)**

**ILL  $2.9 \times 10^9 \text{ n cm}^{-2} \text{ s}^{-1}$  at L/D = 100**

**Converter screen size: 250 x 250 mm**

**Converters:**

**gamma : Gd<sub>2</sub>O<sub>2</sub>S: Tb**

**neutrons: <sup>6</sup>Li:ZnS:Cu, Al, Au (green light)**





**Camera: CCD ORCA-ER (Hammamatsu)**

**Linear resolution: 0.1 mm, time resolution: 1 s**


**Objects: medium size technical devices**

**Processes: water migration in porous systems  
self-diffusion in water**

## Modeling of E2 shield from HZB

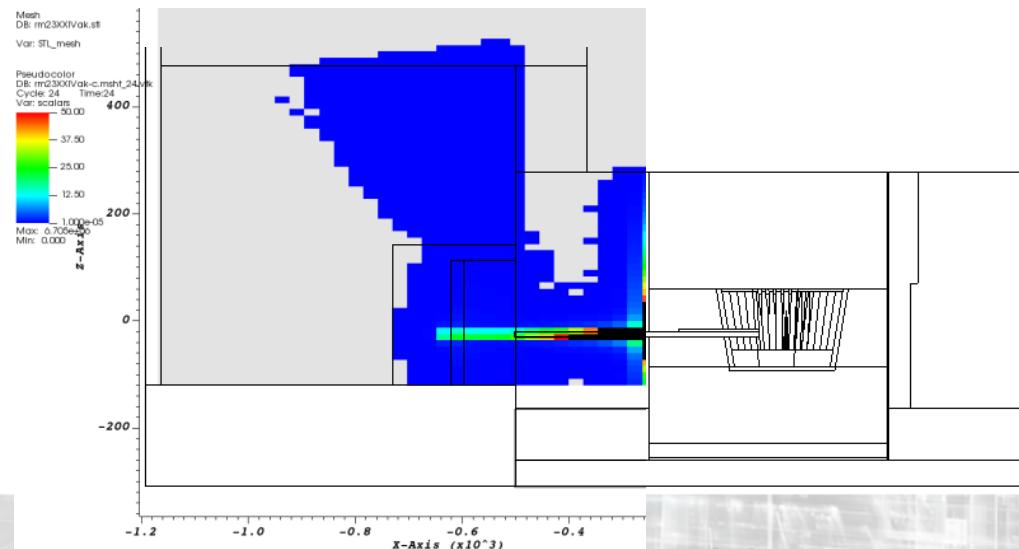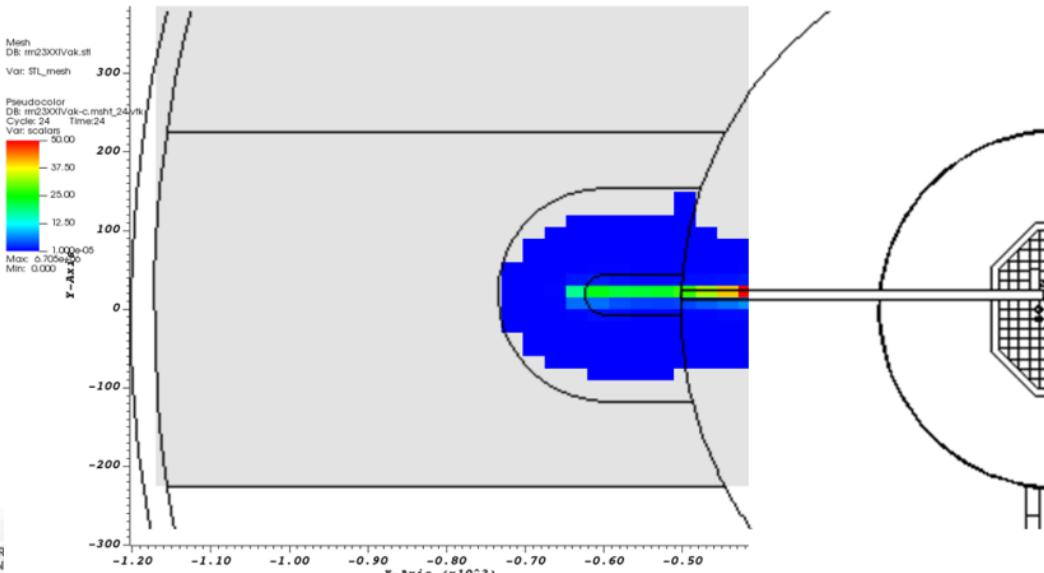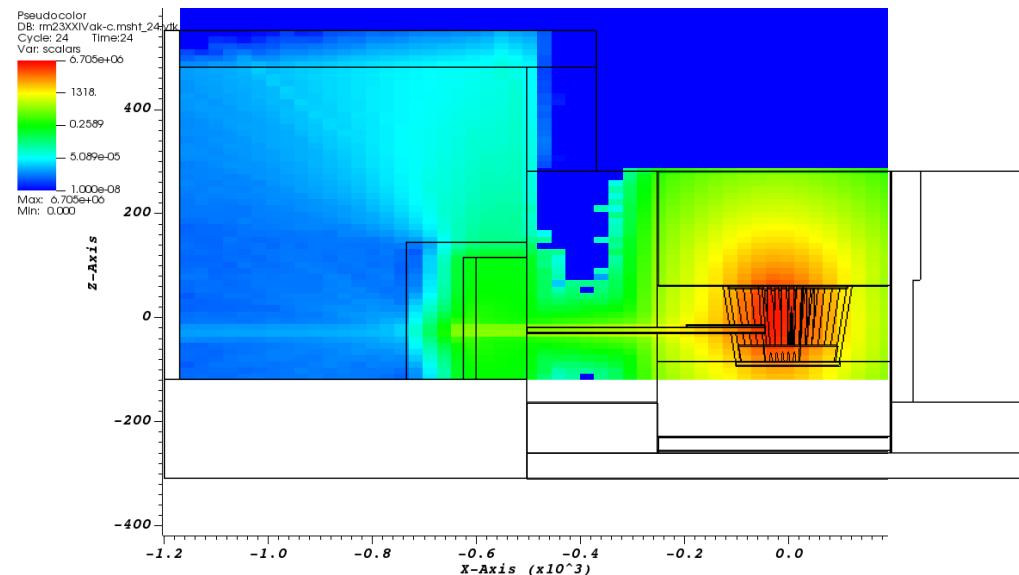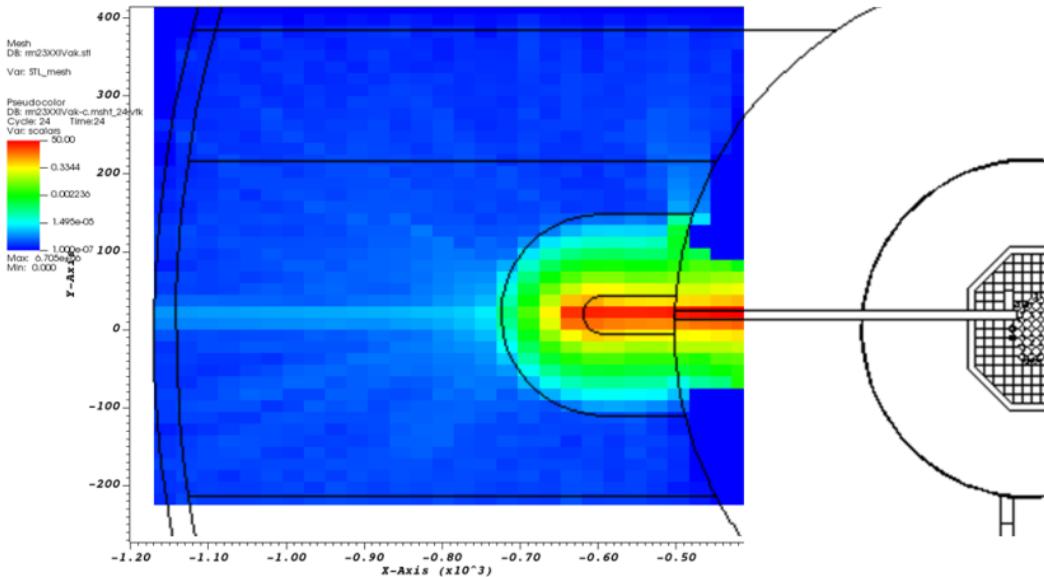

***The main systems (sample and analyser tables, and control) of the E1 spectrometer deployed on the granite floor for training at NCBJ***

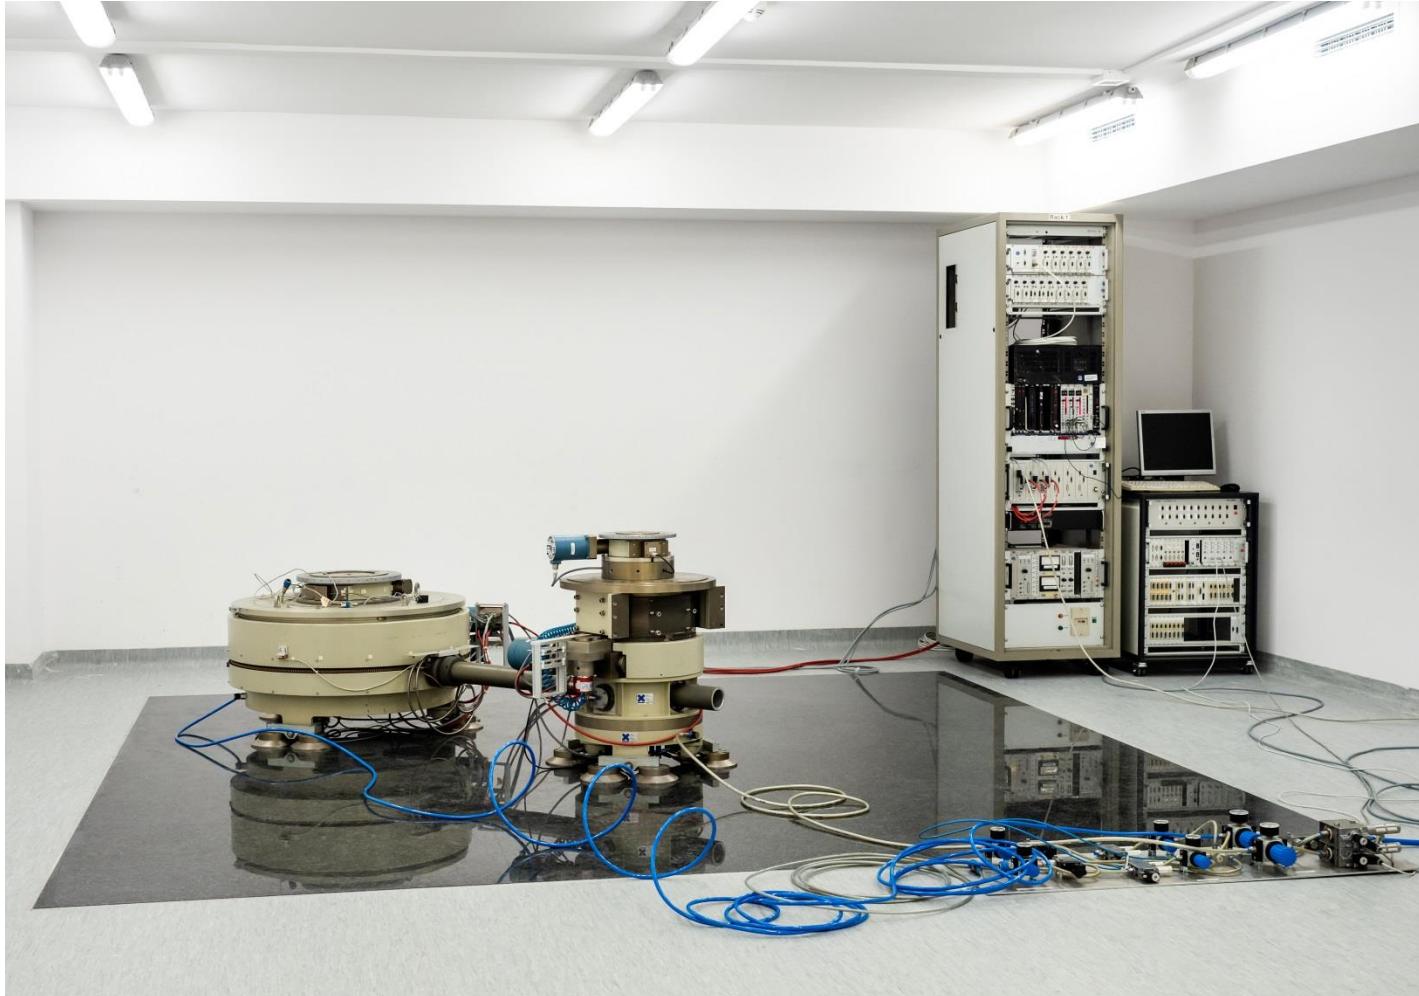

**Concrete floor**



**Granite floor**



**Pressurized air, He recovery, cooling water, N2 and He installations**



## **National Recovery and Resilience Plan (KPO): MNL Maria Neutron Laboratory**

**Eligible expenses:** **25 124 047,06 PLN**

**Funding:** **19 830 000,00 PLN**

- ***Helium recovery and liquefaction station***
- ***Liquid helium and nitrogen dewars***
- ***Adaptation of shields***
- ***CEPH based reliability cluster for storing measurement data***
- ***Computers***
- ***Software***
- ***Modernization of the radiography station***
- ***Modernization of rooms for MNL in the LBM building***



**KRAJOWY  
PLAN  
ODBUDOWY**



**Rzeczpospolita  
Polska**

Sfinansowane przez  
Unię Europejską  
**NextGenerationEU**





# Thank you



NARODOWE  
CENTRUM  
BADAŃ  
JĄDROWYCH  
ŚWIERK

[www.ncbj.gov.pl](http://www.ncbj.gov.pl)